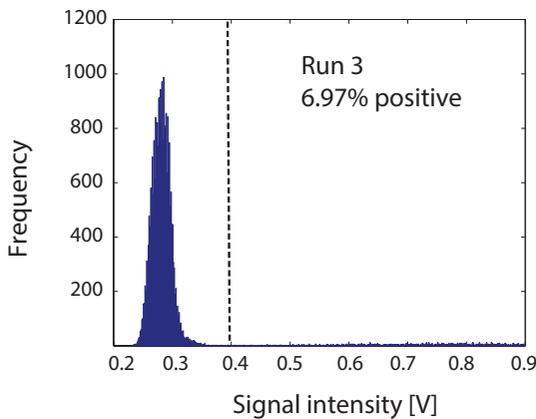
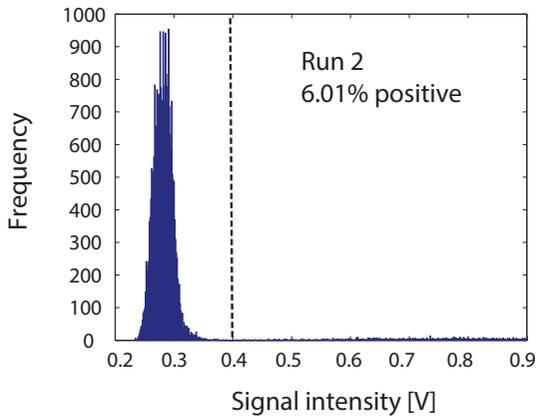
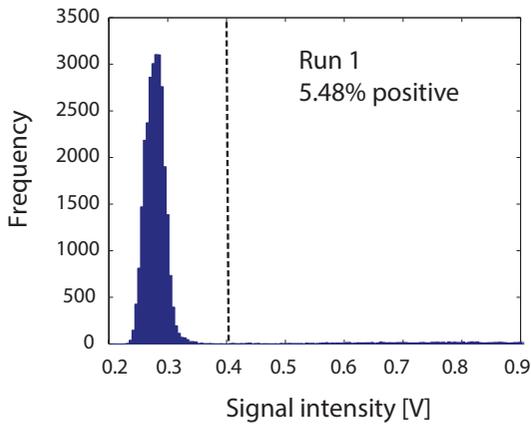
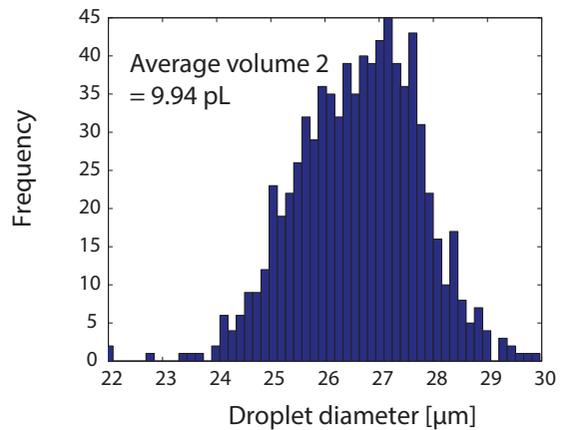
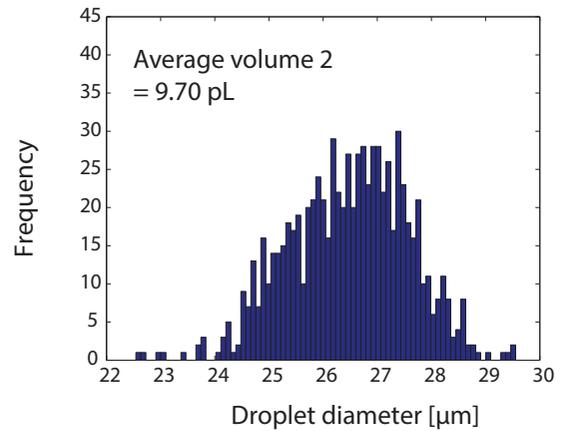
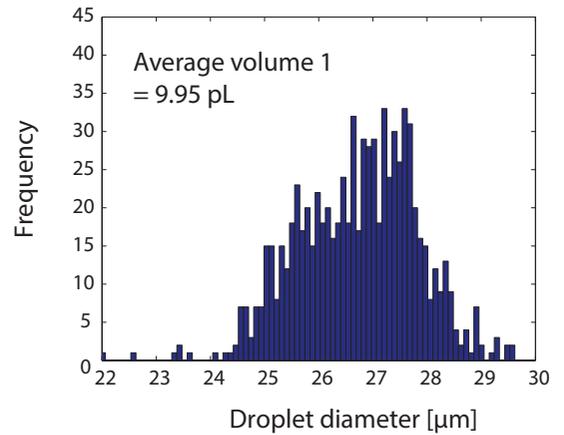


A T4 digital PCR readings**B** T4 droplet size distribution**C**

Run	Positive drops (%)	λ (particles/drop)	Virus conc. (/mL)
1	5.48	0.0798	$8.02 \cdot 10^6$
2	6.01	0.0565	$5.82 \cdot 10^6$
3	6.97	0.0722	$7.26 \cdot 10^6$