

Functionalization of Ti-40Nb Implant Material with Strontium by Reactive Sputtering

Markus Goettlicher¹, Marcus Rohnke¹, Yannik Moryson¹, Jürgen Thomas², Joachim Sann¹, Anja Lode³, Matthias Schumacher³, Romy Schmidt², Stefan Pilz², Annett Gebert², Thomas Gemming², Jürgen Janek¹

¹ Institute of Physical Chemistry & Center of Materials Research, Justus-Liebig-University of Giessen, Heinrich-Buff-Ring 17, 35392 Giessen, Germany

² IFW Dresden, Institute for Complex Materials, Helmholtzstrasse 20, 01069 Dresden, Germany

³ Centre for Translational Bone, Joint and Soft Tissue Research, Faculty of Medicine and University Hospital, Technische Universität Dresden, Fetscherstrasse 74, 01307 Dresden, Germany

X-ray diffraction pattern of surface coating

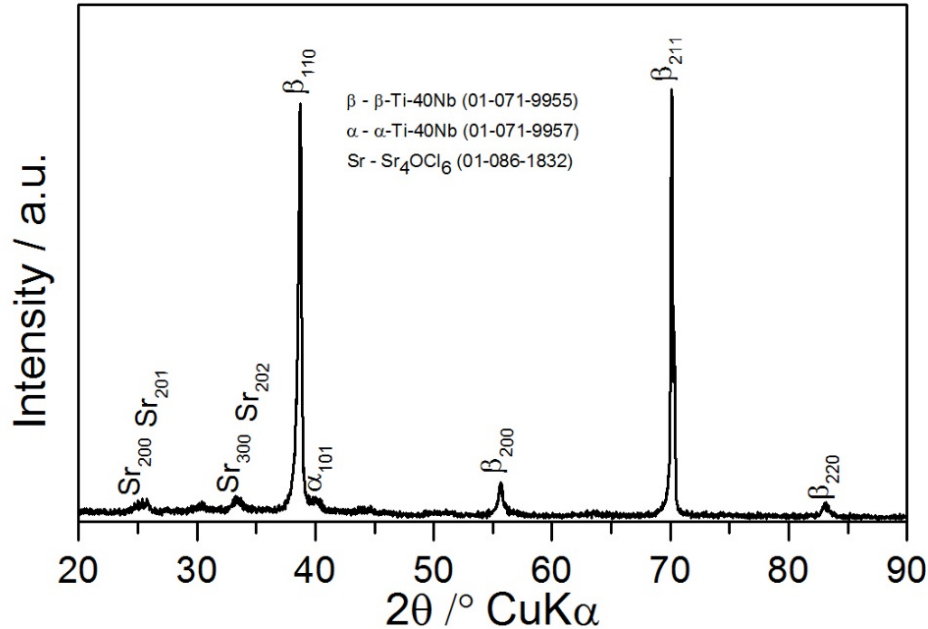


Fig. 1: Grazing incidence diffraction pattern of the deposited layer, incidence angle 2°, in brackets: number of the PDF (powder diffraction file) retrieved from the ICSD database.