

1 **Multiplex immunochromatographic detection of OXA-48, KPC and NDM carbapenemases:**
2 **impact of the inoculum, antibiotics and agar**

3

4 Ahmad Saleh^{a, c}, Stephan Göttig^b and Axel Hamprecht^{a, c}

5

6 a. Institute for Medical Microbiology, Immunology and Hygiene, University Hospital of Cologne,
7 Cologne, Germany

8 b. Institute of Medical Microbiology and Infection Control, Hospital of Johann Wolfgang
9 Goethe-University, Frankfurt am Main, Germany

10 c. DZIF (German Centre for Infection Research), partner site Cologne-Bonn

11


12

13 **Supplementary Data**

14

15

16

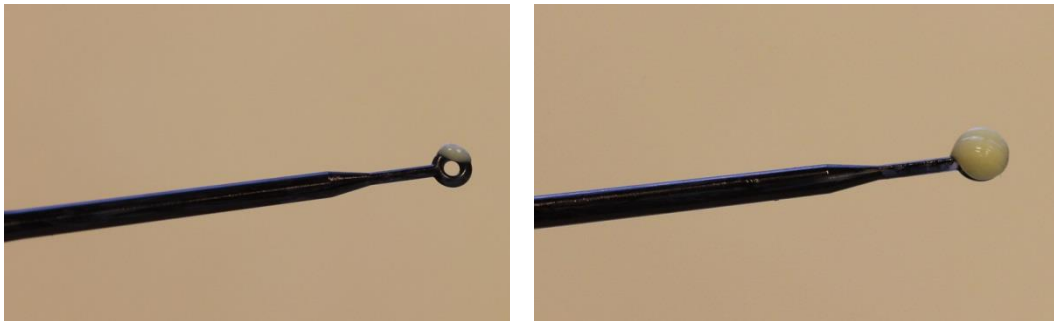

17

18

19 **FIG S1:**

20 Incorrect inoculum (left) vs. correct inoculum (right). A full 1 μ l loop is required to achieve the highest
21 sensitivity, especially for NDM.