


## Additional file 2-verification of antibodies

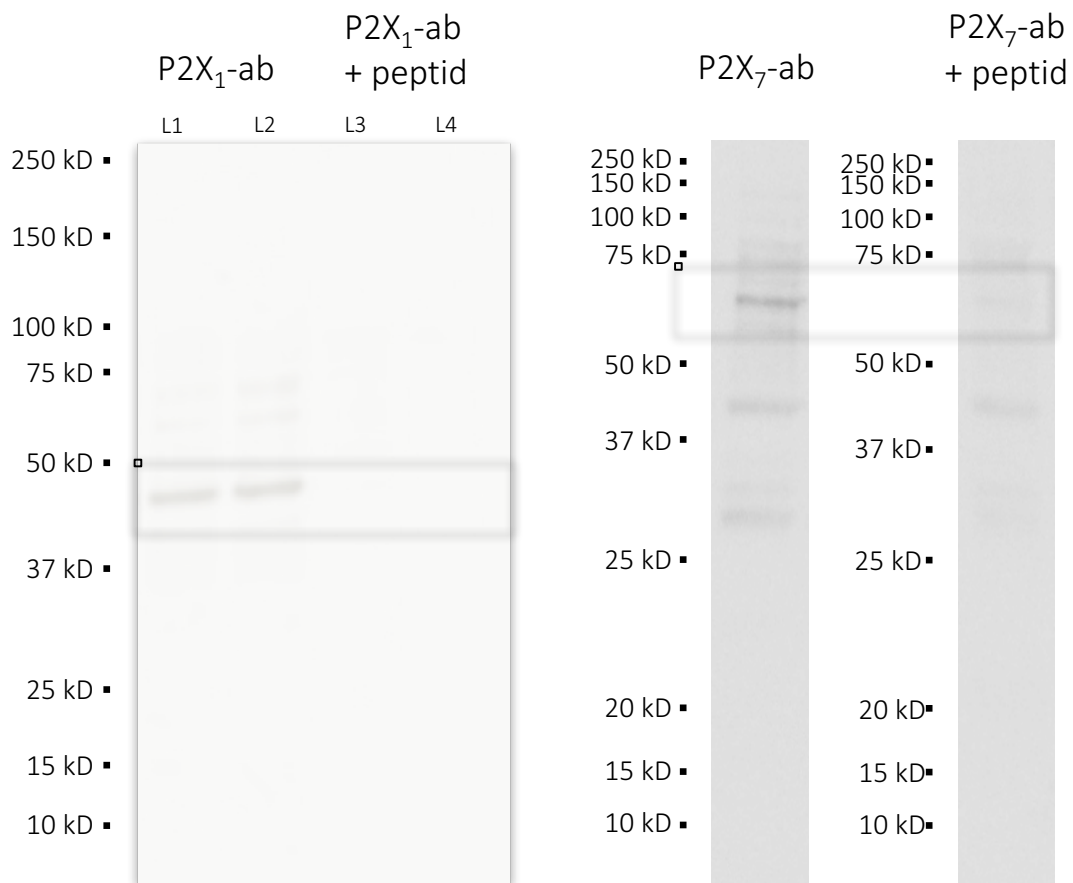

### Additional file 2

Immuno-blot with the P2X<sub>1</sub> and P2X<sub>7</sub> antibodies used for flow cytometric detection of the P2 receptors on the erythrocytes, with or without peptide preadsorption.