



S. aureus erythromycin


SFF=15




SFF=40




SFF=70




SFF=100





SFF=150



SFF=200



SFF=250

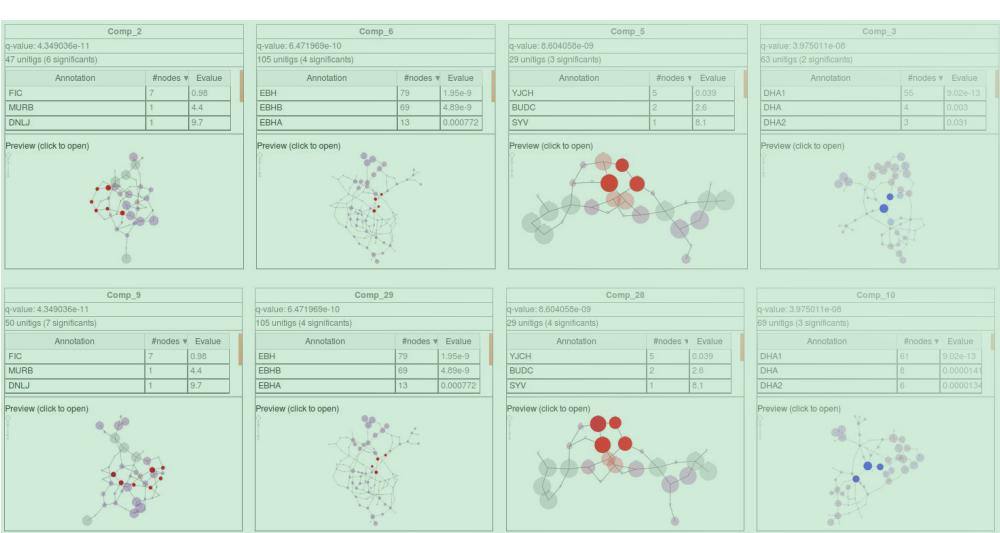

The raw DBGWAS results with the different values for SFF, which are summarised in this figure, are available at http://pbil.univ-lyon1.fr/datasets/DBGWAS_support/experiments/index.html#DBGWAS_all_results_different_SFF