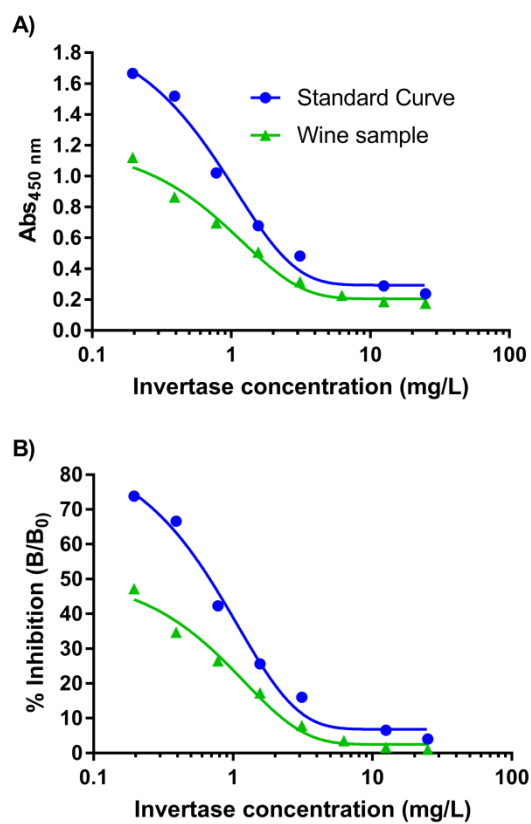


**Appendix A**


**Figure S1:** Calibration curve prepared with serial dilutions of yeast invertase (Standard curve, in blue) and curve prepared from a serial dilution for the determination of MPs content in a sparkling wine sample (in green). Data are expressed as Absorbance measured at 450 nm (A) and as % of inhibition expressed as  $B/B_0$  (B).