




Supplementary Figure 1 : Bioanalyzer electropherograms of the libraries. Not available for CTRL5 and CTRL6.

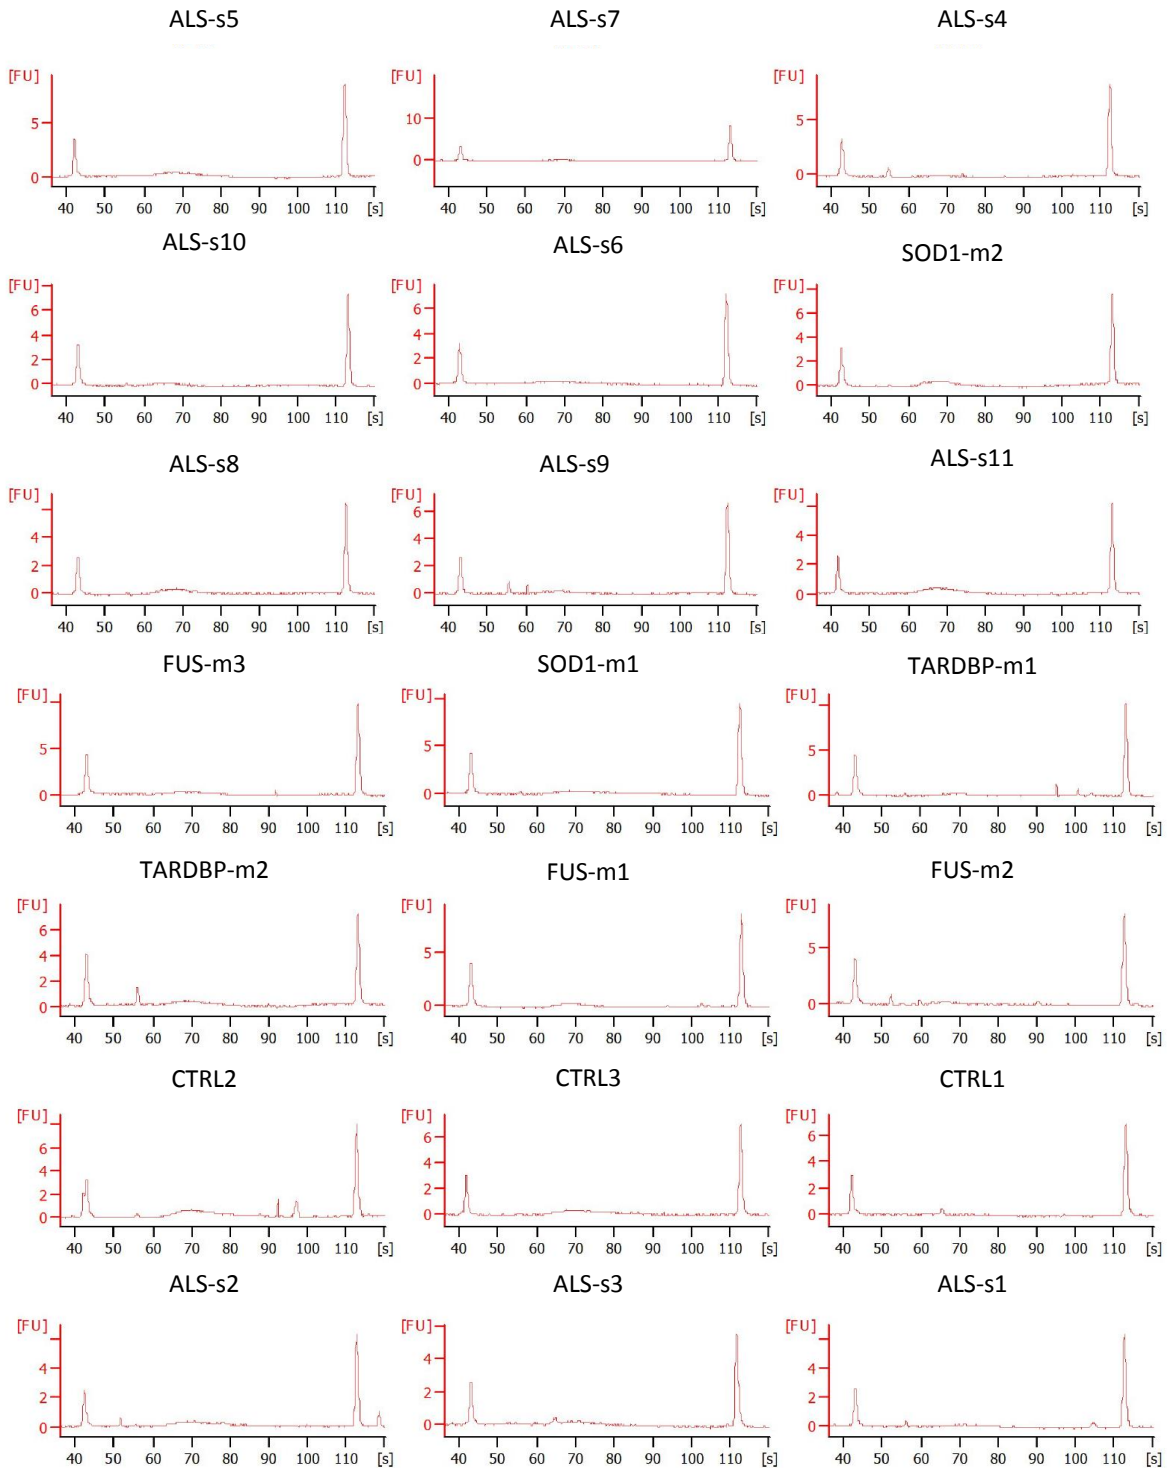


ALS-s15

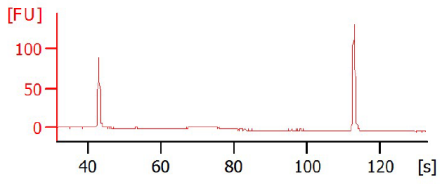


ALS-s16

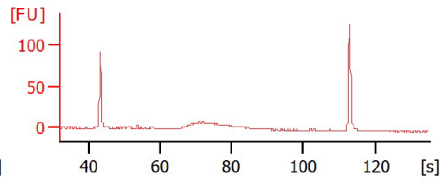


SOD1-m3

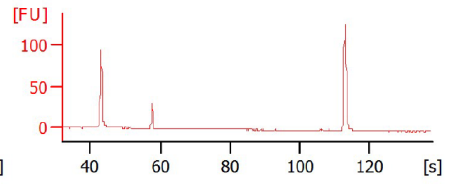


ALS-s13

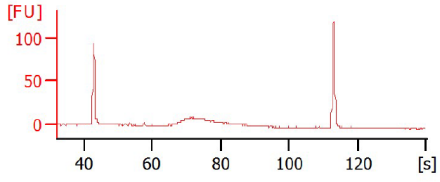


ALS-s12

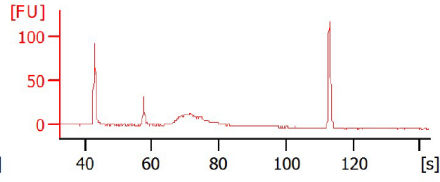

VCP-m1

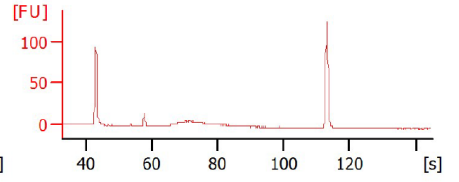

CTRL7

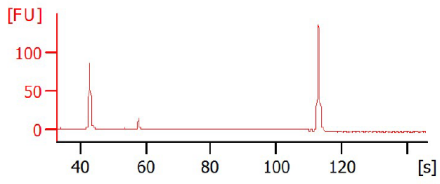

CTRL4

