

Figure S1. Scoring template for InBios ChagasDetect Plus readings

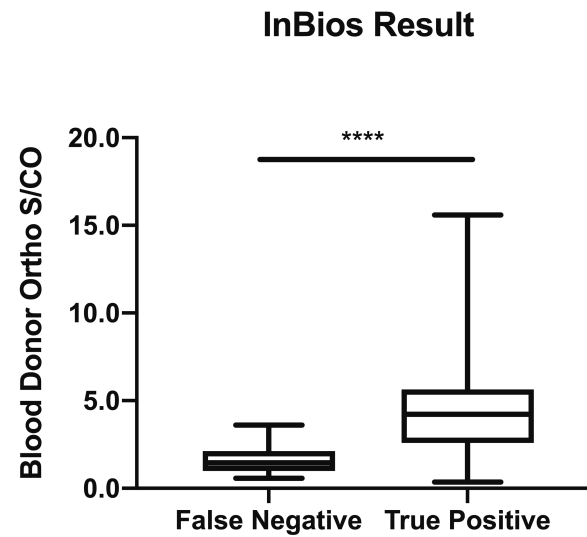
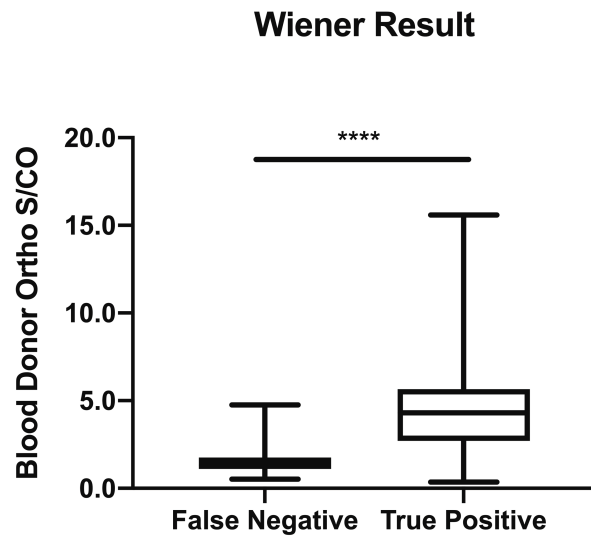
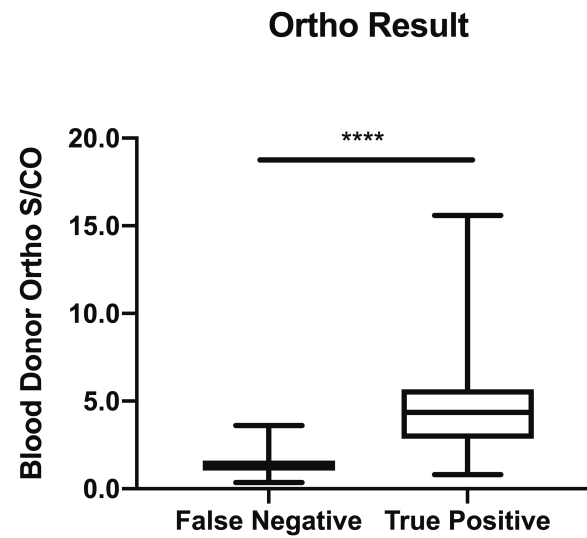
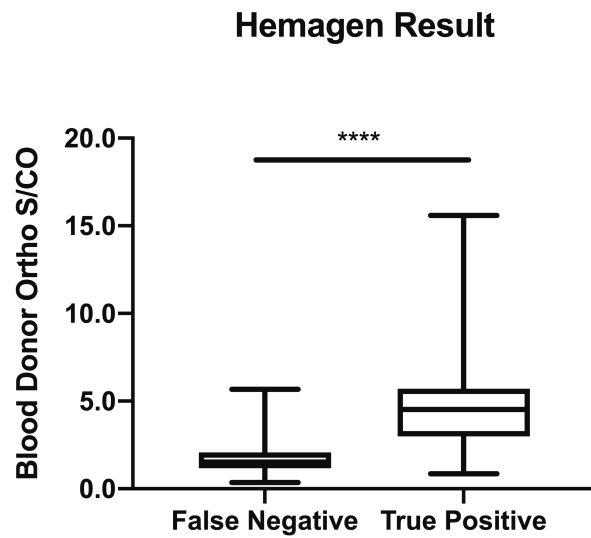


Figure S2. Blood donor Ortho signal-to-cutoff (S/CO) distribution for specimens with false negative and true positive designation by test as compared to blood donor status. ****p<0.0001