

Original gel images contained in the manuscript's Figure 3.

M: The 1-kb DNA ladder.

X: Lanes not included in the manuscript's Fig. 3.


S: The strain #36 was used as the standard strain and included in every experiment as a control.

Date of each run was shown above.

KODAK 1D Image Analysis Software (v. 3.6) was used to capture the images.


20180302

M **36** X X **18 19 20** X

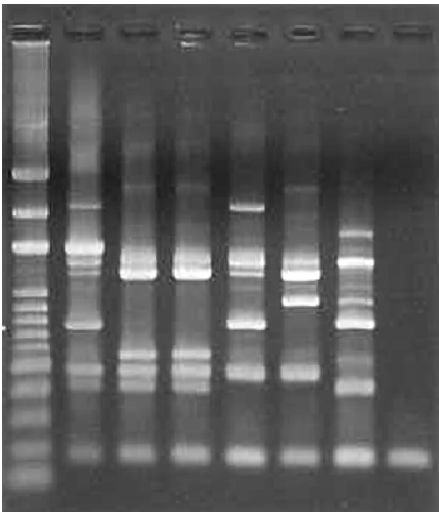


20180306

M **S** **5 8 9 11** X **2 3 4 21** X **17 31 40** X X

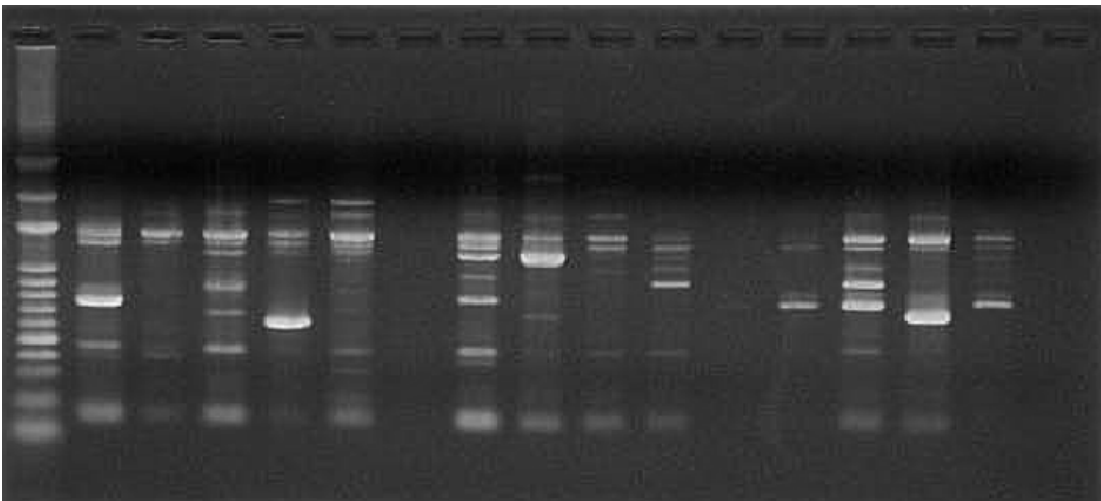


20180312

M **S** 1 7 10 13 14 15 X X X X 24 26 29 16 22

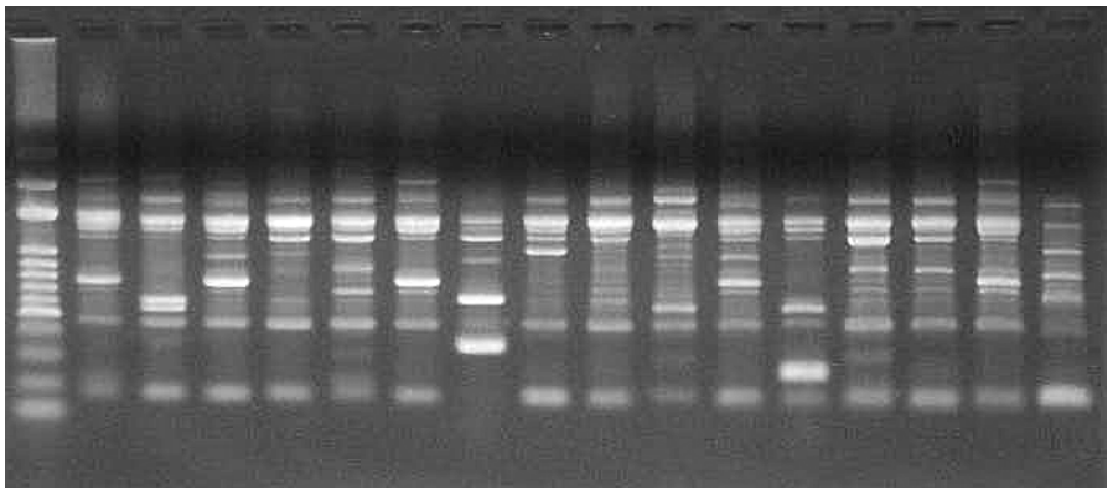


20180314

M **S** X X X 23 25 27 X X X 30 X X X 28 X

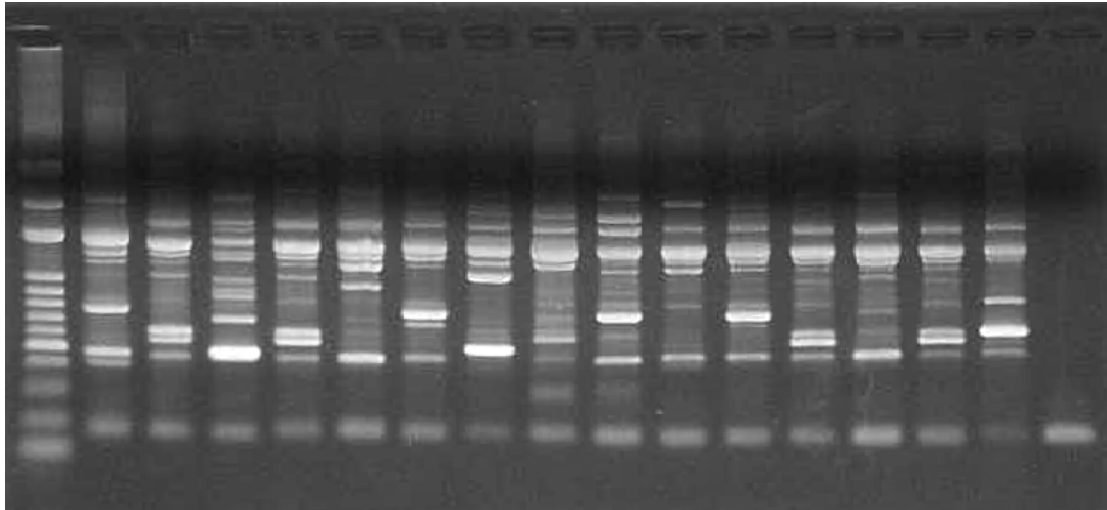


20180319

M **S** X X 33 X X X X 41 X X X X X X X

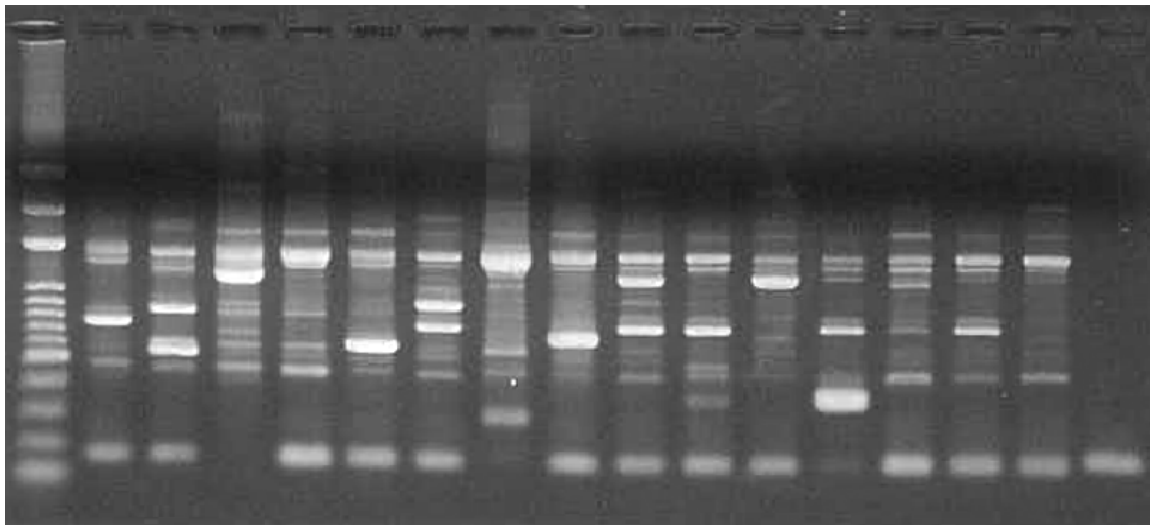


20180321

M **S** 39 X X X X X

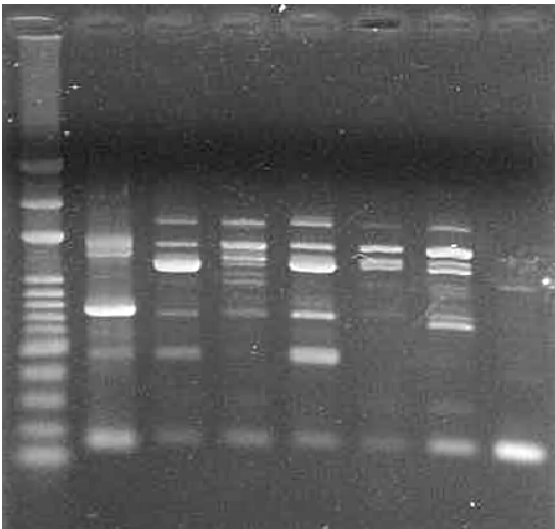

20180322

M **S** 12 32 34 37 35 38 42 43 45 44 46 X X X X

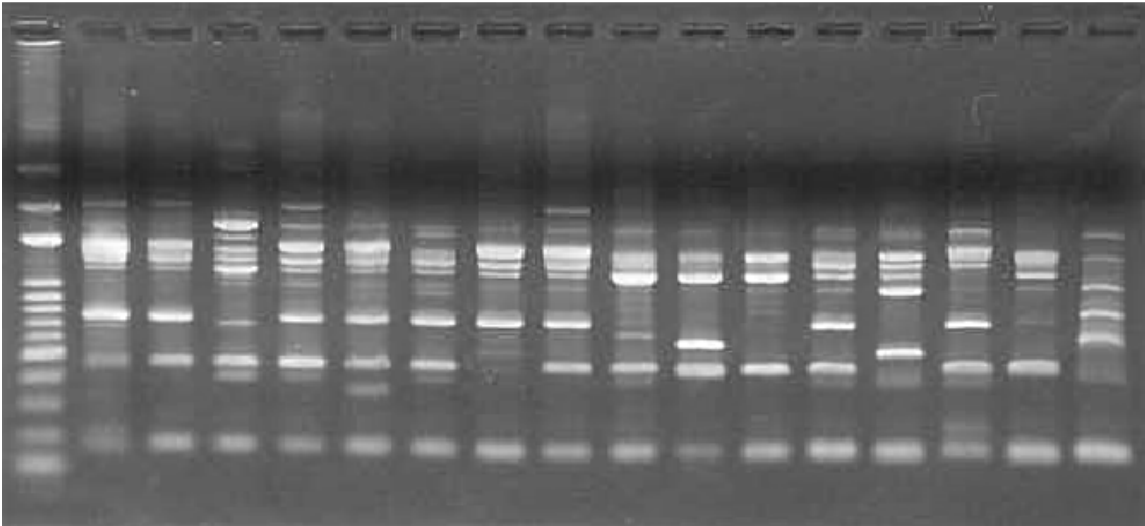

20180419

M **S** X 6 X X X X X X X X X X X X

