


Supplemental Appendix 1: Timeline of program and evaluation elements

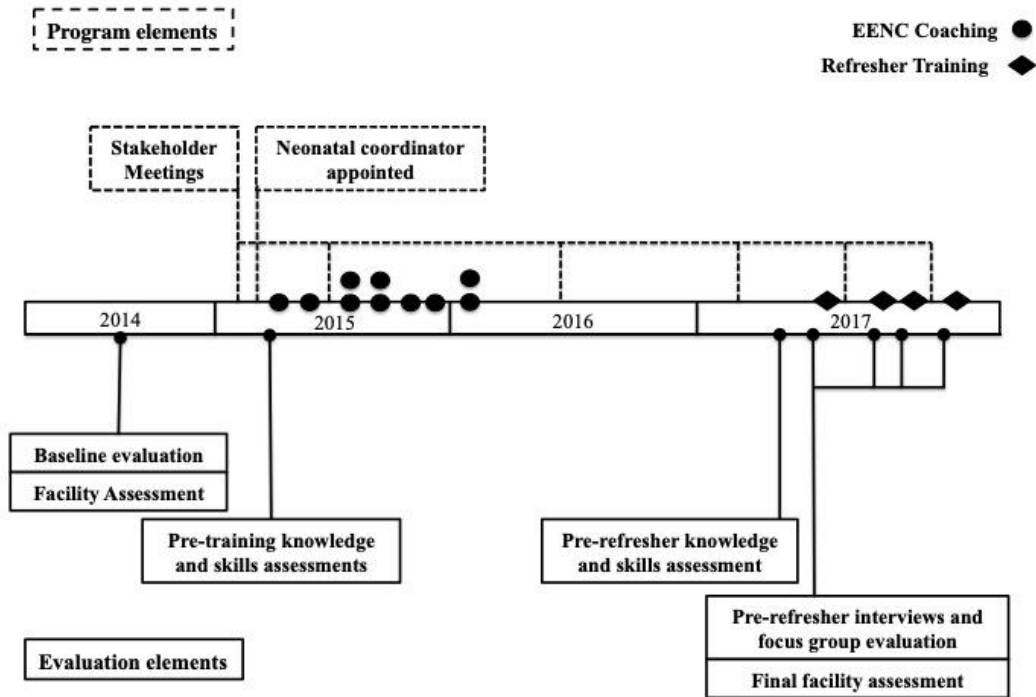

## Supplemental Appendix 2: Minimum Neonatal Equipment Standards

---

<b>Item Description</b>	<b>Quantity for 10 bed unit (NRH)</b>	<b>Quantity for 6 bed unit (Provincial Hospital)</b>
<b>General</b>		
Resuscitation trolley (radiant warmer, fixed height, drawers, oxygen tank attachment)	3	2
Newborn self-inflating bag/mask resuscitation device 50ml	6	4
Portable electronic suction machine	3	2
Neonatal Cots (+Bedding/Blankets)	12	6
Wall thermometer	1	1
HemoCue Glucose monitors	3	1
Electronic Weighing Scale	2	1
<b>Oxygen</b>		
Oxygen Concentrator	4	2
Paediatric oxygen tubing		
Paediatric oxygen cannulae		
Portable Neonatal/Infant Oximeter (+ probes)	6	3
<b>Monitoring</b>		
Apnoea monitor	4	2
ECG machine	1	1
Neonatal Monitor (HR,SpO2, ECG, RR, Temp)	6	2
Digital Thermometer	6	3
Timing Device/Clock	2	1