


Supplementary Figure 2

Johannesburg Validation Cohort

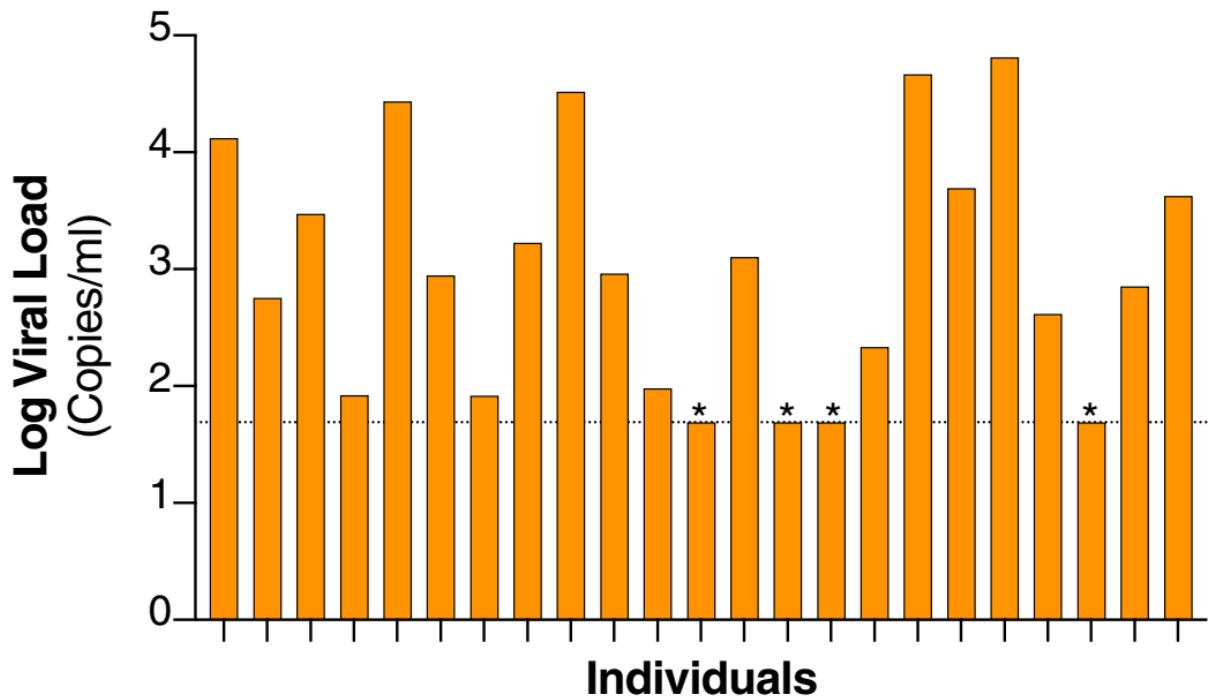

*Below Limit of detection (50 copies/ml)