



Raw Image
for Figure 2A

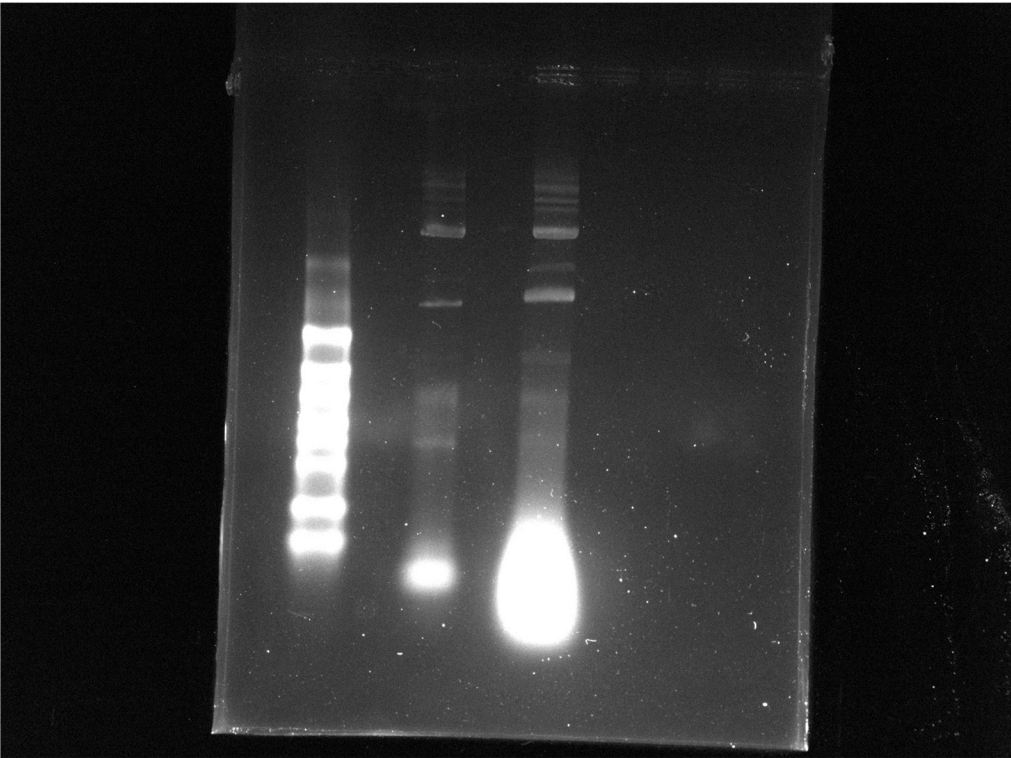

Raw Image
for Figure 2B

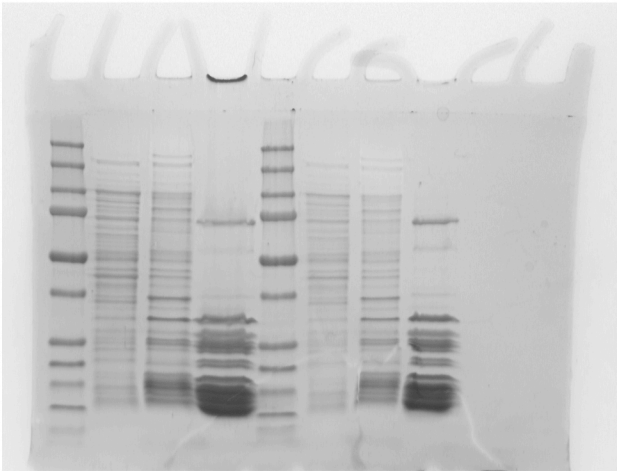

Biorad gel Imaging system was used to capture the gel images