
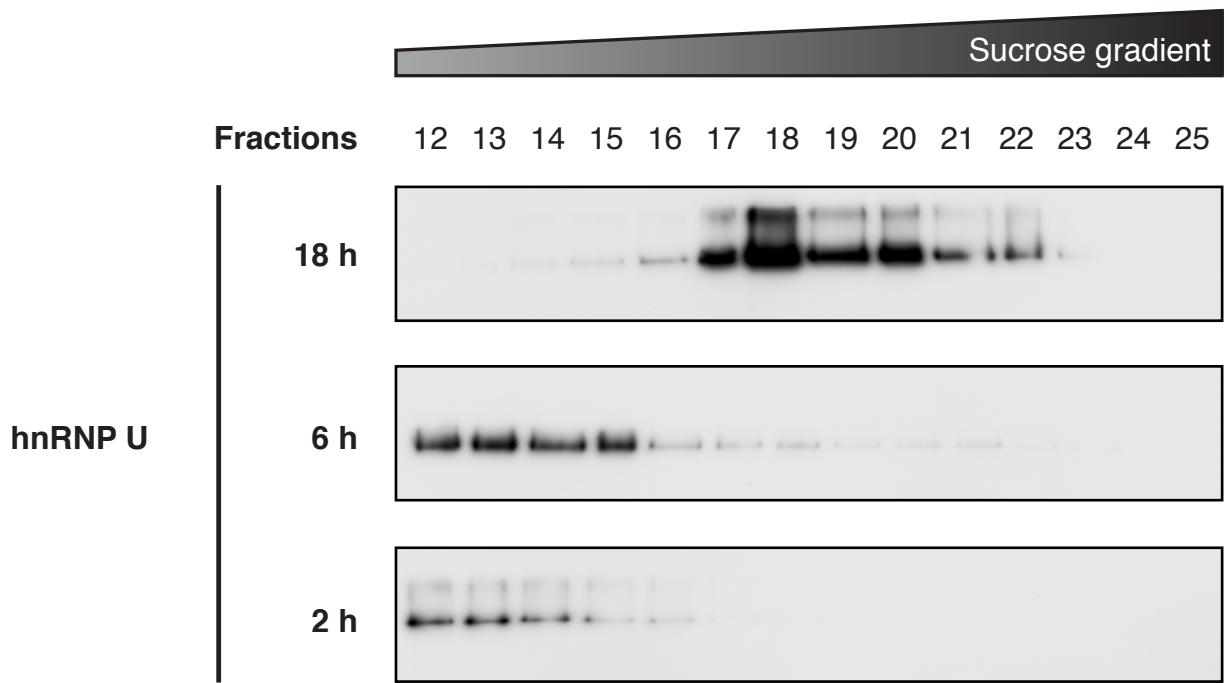
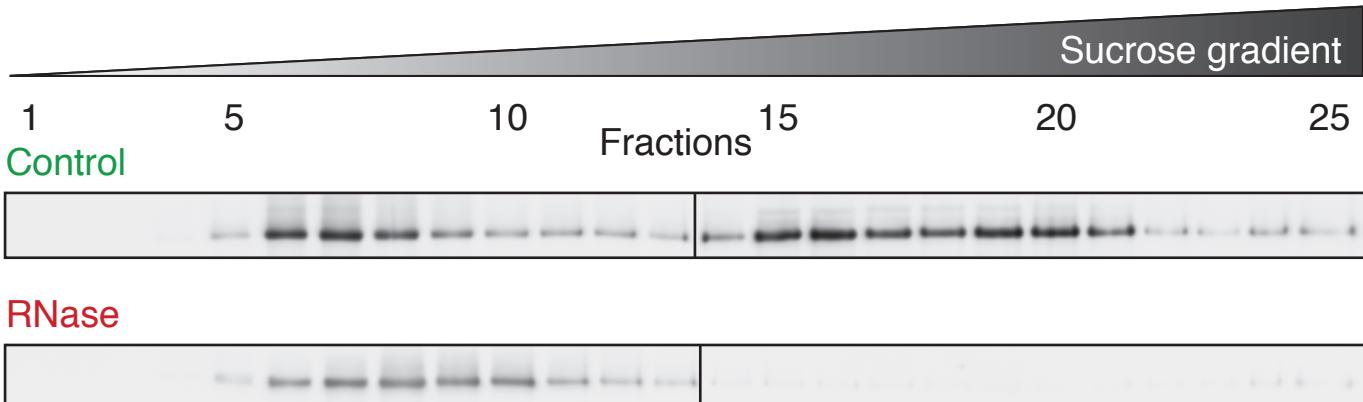
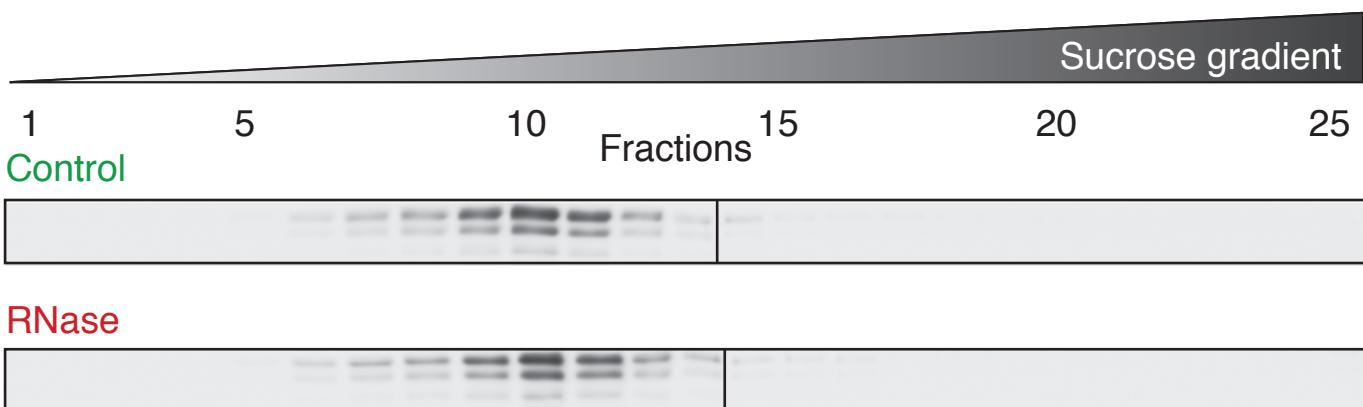
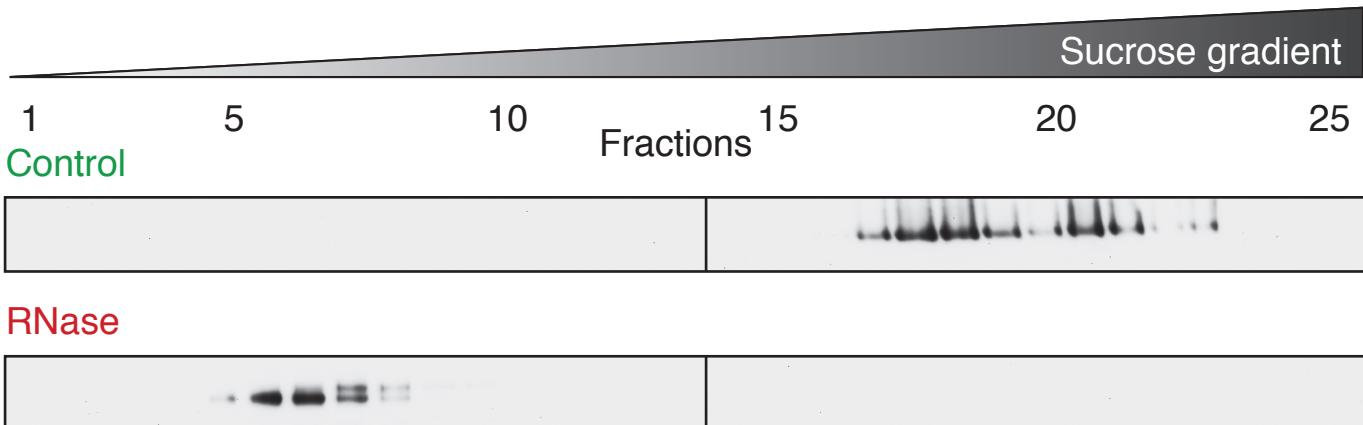



Caudron-Herger et al. Supplementary Fig. 1

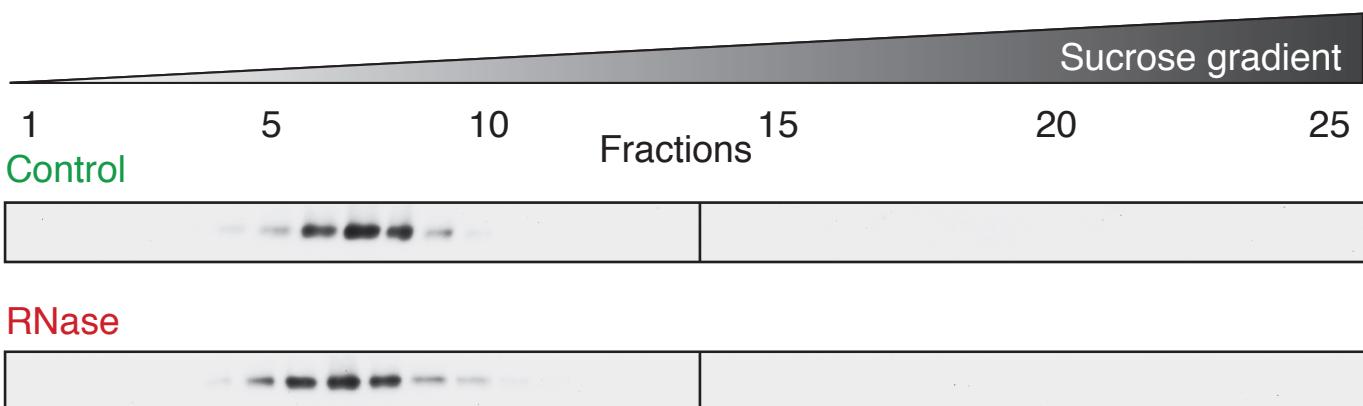


Caudron-Herger et al. Supplementary Fig. 2

a**b****c****d**

Settings for measurements in ImageJ

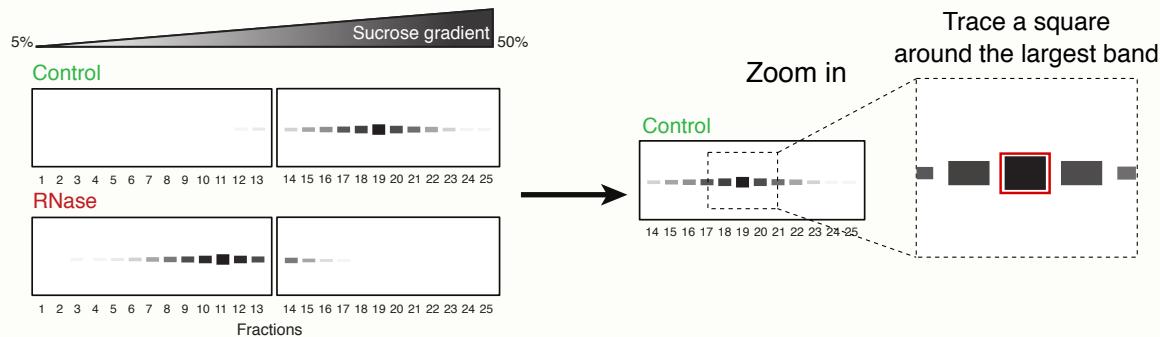

Measurement of band intensities

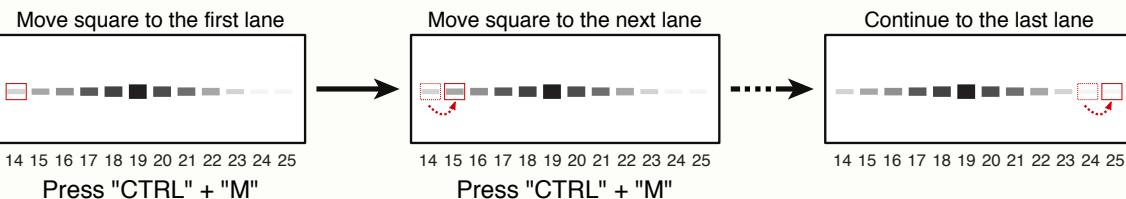


Data processing

Save data and export

	Area	Intensity
1	1800	2605328
2	1800	6354878
...
25	1800	1265489

Repeat on all blots

Normalization

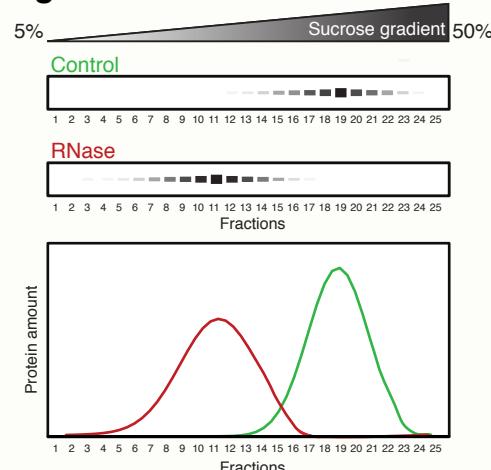

Caudron-Herger et al. Supplementary Fig. 4