


Supplementary Data

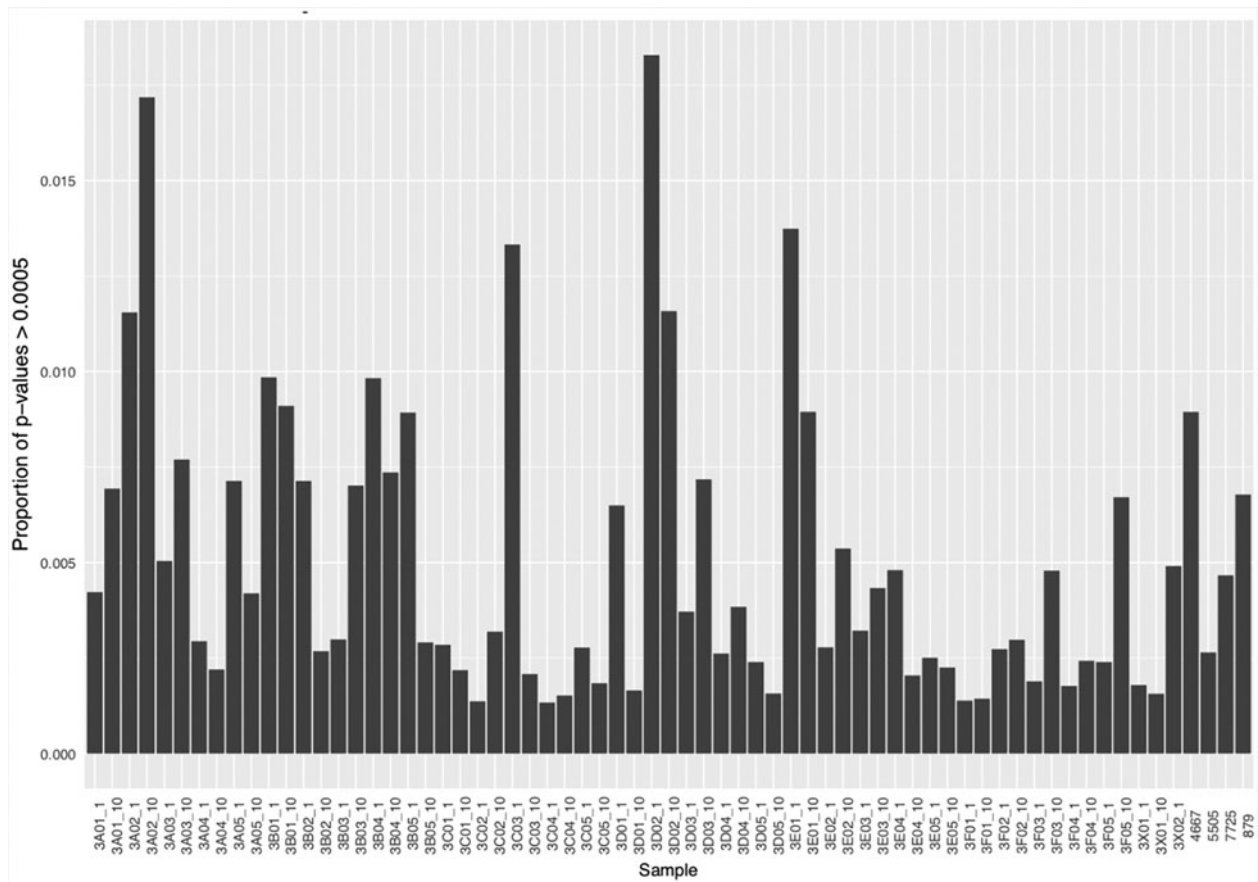

SUPPLEMENTARY FIG. S1. Quality control, detection p value. Showing the proportion of probes with poor quality ($p > 0.0005$) probes for each biological sample. All samples had high-quality data, with at least 98% of probes passing criteria.