

Article

Flexible Textile-Based Pressure Sensing System Applied in the Operating Room for Pressure Injury Monitoring of Cardiac Operation Patients

De-Fen Shih ^{1,†}, Jyh-Liang Wang ^{1,2,†}, Sou-Chih Chao ^{1,2}, Yin-Fa Chen ³, Kuo-Sheng Liu ⁴, Yi-Shan Chiang ⁵, Chi Wang ^{5,6}, Min-Yu Chang ^{5,7}, Shu-Ling Yeh ^{5,8}, Pao-Hsien Chu ⁹, Chao-Sung Lai ^{10,11,12,13}, Der-Chi Shye ^{1,2}, Lun-Hui Ho ^{5,8,*} and Chia-Ming Yang ^{3,10,11,14}

¹ eBio Technology Inc., Xinzhuang, New Taipei City 242, Taiwan; stephanie@ebio-health.com (D.-F.S.); joewang@mail.mcut.edu.tw (J.-L.W.); willson@ebio-health.com (S.-C.C.); DCS19680323@gmail.com (D.-C.S.)

² Department of Electronic Engineering, Ming Chi University of Technology, New Taipei 243, Taiwan

³ Institute of Electro-Optical Engineering, Chang Gung University, Taoyuan 333, Taiwan; chenbearfa@gmail.com (Y.-F.C.); cmyang@mail.cgu.edu.tw (C.-M.Y.)

⁴ Department of Cardiac Surgery, Chang Gung Memorial Hospital, Linkou 333, Taiwan; liuks@me.com

⁵ Department of Nursing, Linkou Chang Gung Memorial Hospital, Linkou 333, Taiwan; robelaec@cgmh.org.tw (Y.-S.C.); gigy@cgmh.org.tw (C.W.); yu@cgmh.org.tw (M.-Y.C.); q22122@cgmh.org.tw (S.-L.Y.)

⁶ Department of Nursing, Chang Gung University, Taoyuan 333, Taiwan

⁷ Department of Nursing, Oriental Institute of Technology, New Taipei City 220, Taiwan

⁸ Department of Nursing, Chang Gung University of Science and Technology, Taoyuan 333, Taiwan

⁹ Department of Cardiology, Chang Gung Memorial Hospital, School of Medicine, Chang Gung University, 199 Tung Hwa North Road, Taipei 105, Taiwan; pchu@cgmh.org.tw

¹⁰ Department of Electronic Engineering, Chang-Gung University, Taoyuan 333, Taiwan; cslai@mail.cgu.edu.tw

¹¹ Biosensor Group, Biomedical Engineering Research Center, Chang Gung University, Taoyuan 333, Taiwan

¹² Department of Nephrology, Chang Gung Memorial Hospital, Linkou 333, Taiwan

¹³ Department of Materials Engineering, Ming-Chi University of Technology, New Taipei City 243, Taiwan

¹⁴ Department of General Surgery, Chang Gung Memorial Hospital, Linkou 333, Taiwan

* Correspondence: ho1180@cgmh.org.tw; Tel: +886-3-3281200 (ext. 2811)

† D.-F. Shih and J.-L. Wang contributed equally to this work.

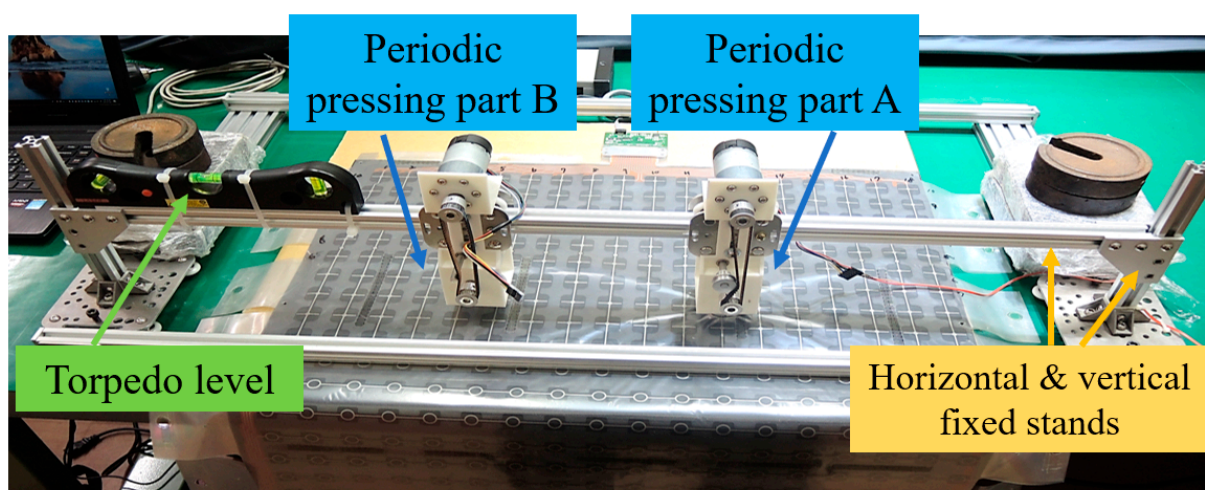


Figure 1. Picture of a regular pressing force by the mechanical setup for the single-pressure sensor.

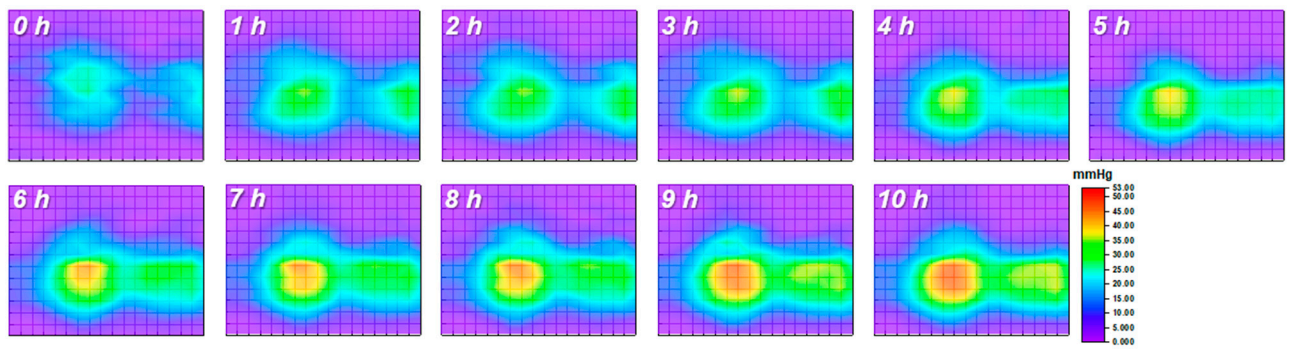


Figure 2. Time-dependent 2D pressure image for a typical patient with low BMI and without pressure injury.



© 2020 by the authors. Licensee MDPI, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons Attribution (CC BY) license (<http://creativecommons.org/licenses/by/4.0/>).