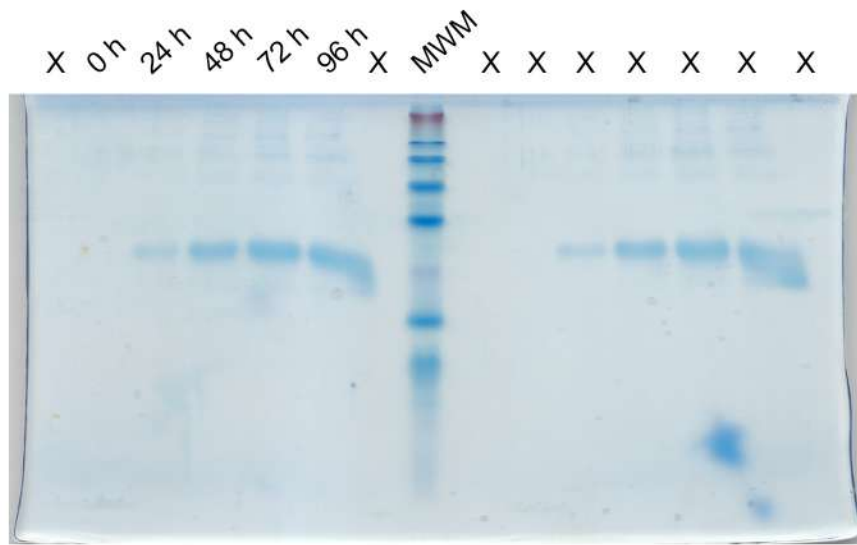Images were obtained using a Canon scanner

Fig 1 panel A
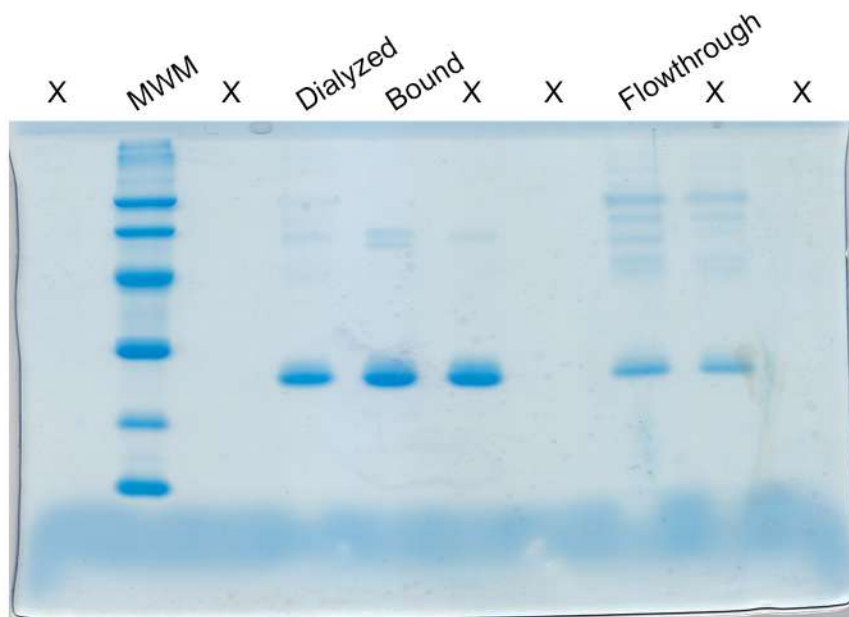

Fig 2 panel B