

Direct measurement of the scattering coefficient: supplement

MARTIN HOHMANN,^{1,2,*} BENJAMIN LENGENFELDER,^{1,2} DANIEL MUHR,¹ MORITZ SPÄTH,^{1,2} MAXIMILIAN HAUPTKORN,¹ FLORIAN KLÄMPFL,^{1,2} AND MICHAEL SCHMIDT^{1,2}

¹*Institute of Photonic Technologies (LPT), Friedrich-Alexander-Universität Erlangen-Nürnberg (FAU), Germany*

²*Erlangen Graduate School in Advanced Optical Technologies (SAOT), Paul-Gordan-Straße 6, 91052 Erlangen, Germany*

**Martin.Hohmann@FAU.de*

This supplement published with The Optical Society on 14 December 2020 by The Authors under the terms of the [Creative Commons Attribution 4.0 License](https://creativecommons.org/licenses/by/4.0/) in the format provided by the authors and unedited. Further distribution of this work must maintain attribution to the author(s) and the published article's title, journal citation, and DOI.

Supplement DOI: <https://doi.org/10.6084/m9.figshare.13274681>

Parent Article DOI: <https://doi.org/10.1364/BOE.410248>

Attachments: Direct measurement of the scattering coefficient

MARTIN HOHMANN^{1,2,*}, BENJAMIN LENGENFELDER^{1,2}, DANIEL MUHR¹, MORITZ SPÄTH^{1,2}, MAXIMILIAN HAUPTKORN¹, FLORIAN KLÄMPFL^{1,2}, MICHAEL SCHMIDT^{1,2}

¹Institute of Photonic Technologies (LPT), Friedrich-Alexander-Universität Erlangen-Nürnberg (FAU), Germany

²Erlangen Graduate School in Advanced Optical Technologies (SAOT), Paul-Gordan-Straße 6, 91052 Erlangen, Germany

Martin.Hohmann@FAU.de

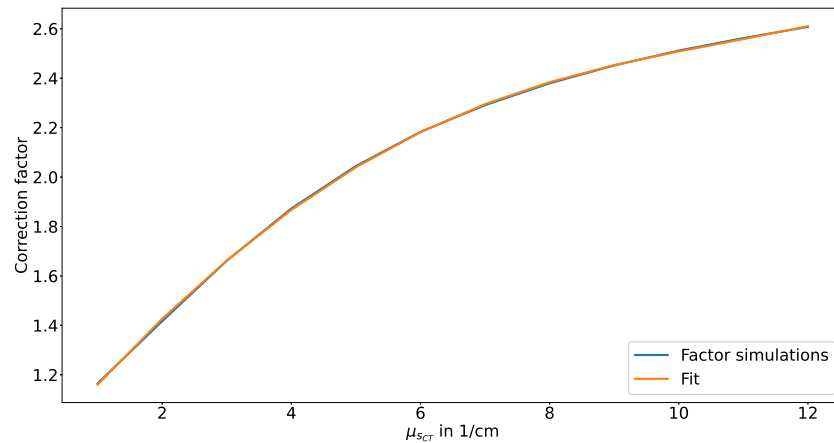


Figure 1: Factor by which TT would be higher for the case of planes with a width and height of 6 cm instead of a cuvette for low absorption coefficients (smaller than $0.01 \frac{1}{cm}$). With this size, nearly all photons can be measured, which are able to pass through. The lower correction factor for low scattering is caused by the fact that not enough light is scattered to affect the result.