


On-line Table: Agreement among semiautomatic packages

	Philips	TeraRecon	Siemens
Mean paired difference degree of stenosis \pm SD (Bland-Altman 95% limits of agreement)			
3mensio	-3.5 \pm 13 (-30-22)	0.55 \pm 13 (-26-27)	2.7 \pm 11 (-18-24)
Philips		5.7 \pm 14 (-22-33)	5.1 \pm 15 (-24-34)
TeraRecon			-1.1 \pm 17 (-33-31)
ICC (95% CI)			
3mensio	0.88 (0.83-0.91)	0.85 (0.80-0.89)	0.90 (0.85-0.93)
Philips		0.84 (0.72-0.90)	0.80 (0.68-0.87)
TeraRecon			0.82 (0.76-0.87)

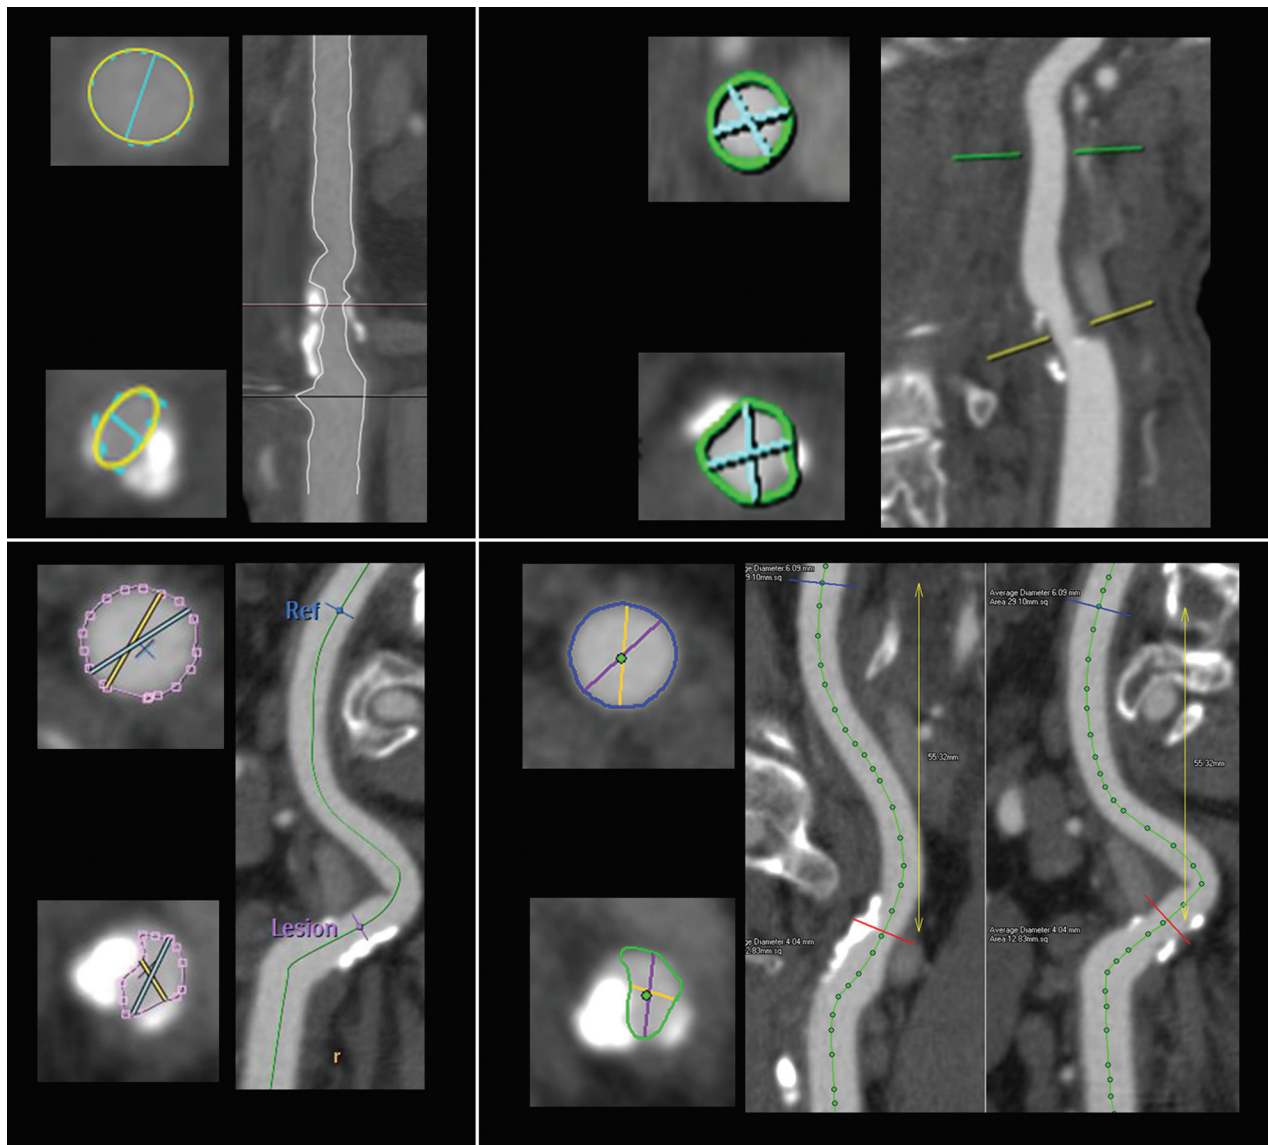

ON-LINE FIG 1. Examples of semiautomatic measurements with 3mensio (upper left corner), Siemens (upper right corner), TeraRecon (lower right corner), and Philips (lower left corner).