

Supplementary Information

Sensitive Impedimetric Detection of Troponin I with Metal-Organic Framework Composite Electrode

Arushi Gupta^{1,2}, Sandeep Kumar Sharma³, Vivek Pachauri⁴, Sven Ingebrandt⁴, Suman Singh¹, Amit L Sharma^{1,2}, Akash Deep^{1,2*}

¹Central Scientific Instruments Organisation (CSIR-CSIO), Sector 30-C, Chandigarh, India;

²Academy of Scientific and Innovative Research (AcSIR-CSIO), Ghaziabad-201002,

Chandigarh, India; ³Department of Physics, Sri Guru Gobind Singh College, Sector 26,

Chandigarh, India; ⁴IWE1 –Institut für Werkstoffe der Elektrotechnik1, RWTH Aachen

University, Germany

Correspondence: *dr.akashdeep@csio.res.in (AD)*

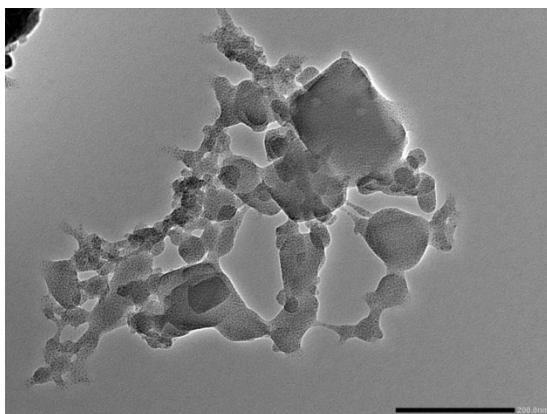


Figure S1. TEM image of Cu₃(BTC)₂

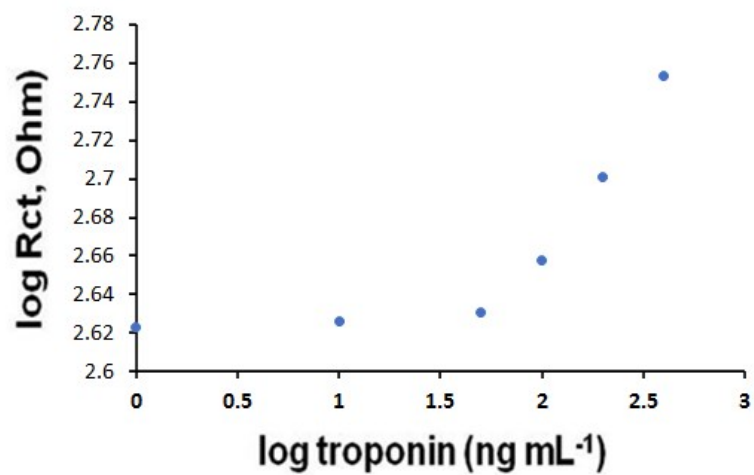


Figure S2. Detection of cTnI with a reference Ab/PANI biosensor, the sensor did not produce any discernible response below 50 ng/mL