



## A) Standard sample preparation \*

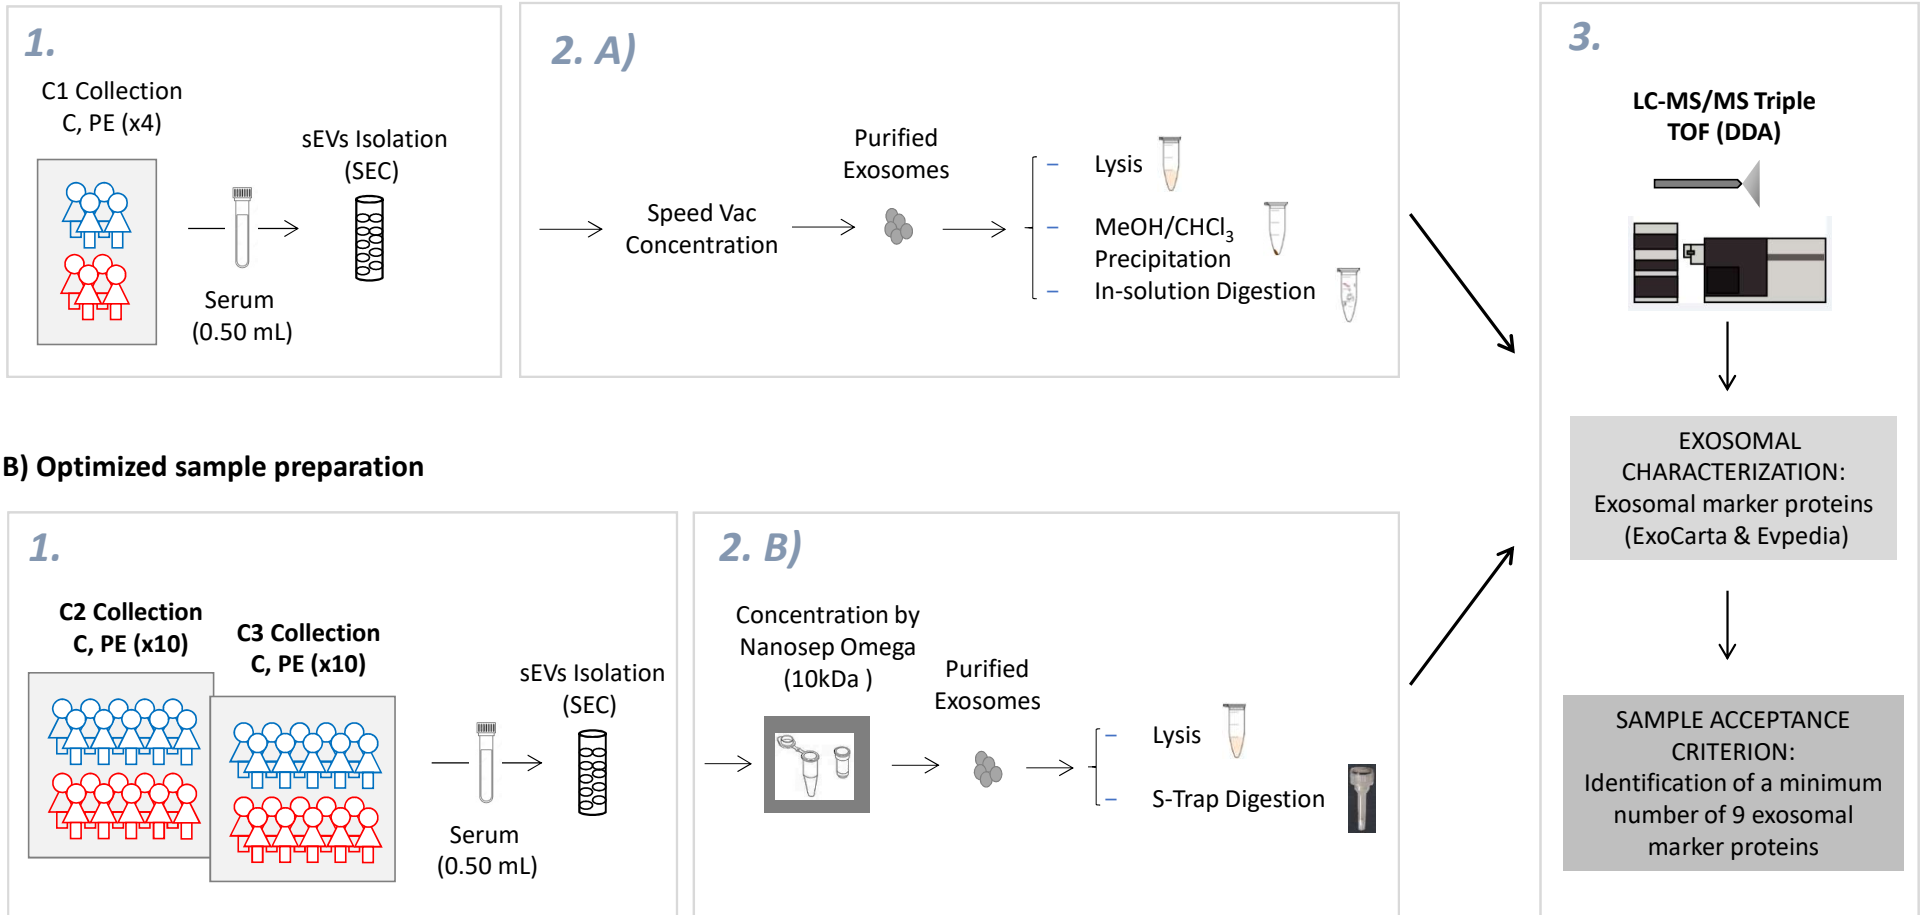

## B) Optimized sample preparation

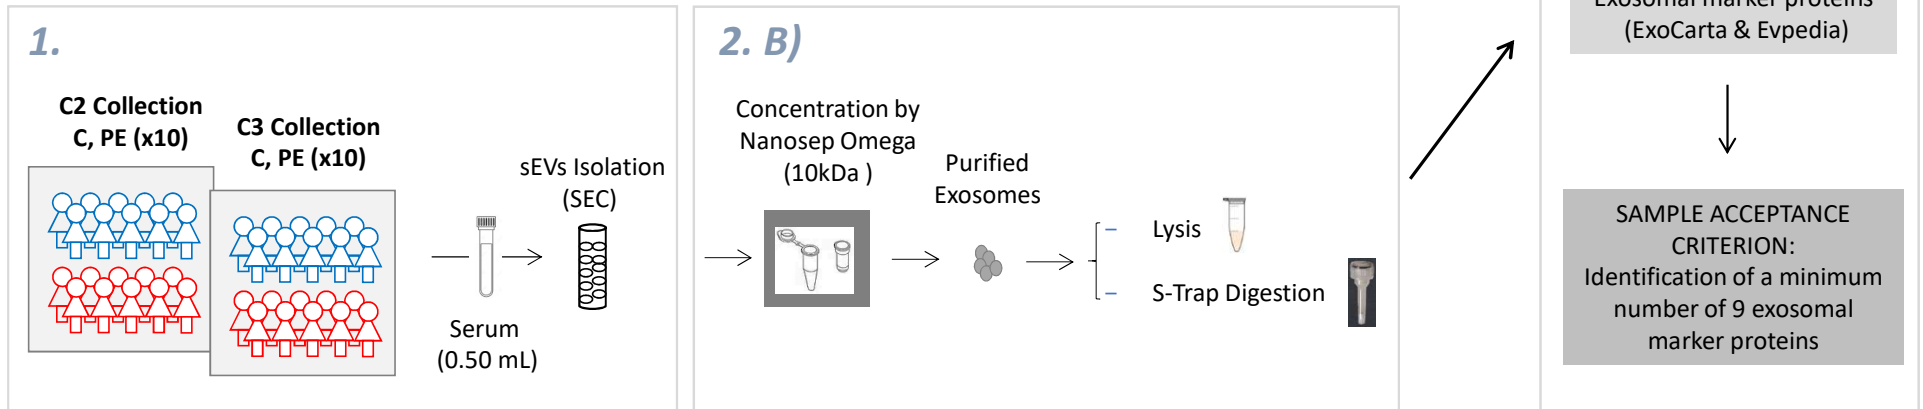

\* C4 collection (11 control and 11 preeclampsia samples), only used for PZP validation by MRM, also followed the standard sample preparation