

Figure (S1) calibration curves of A) sensor 1 B) sensor 2 and C) sensor 3 at different temperatures.

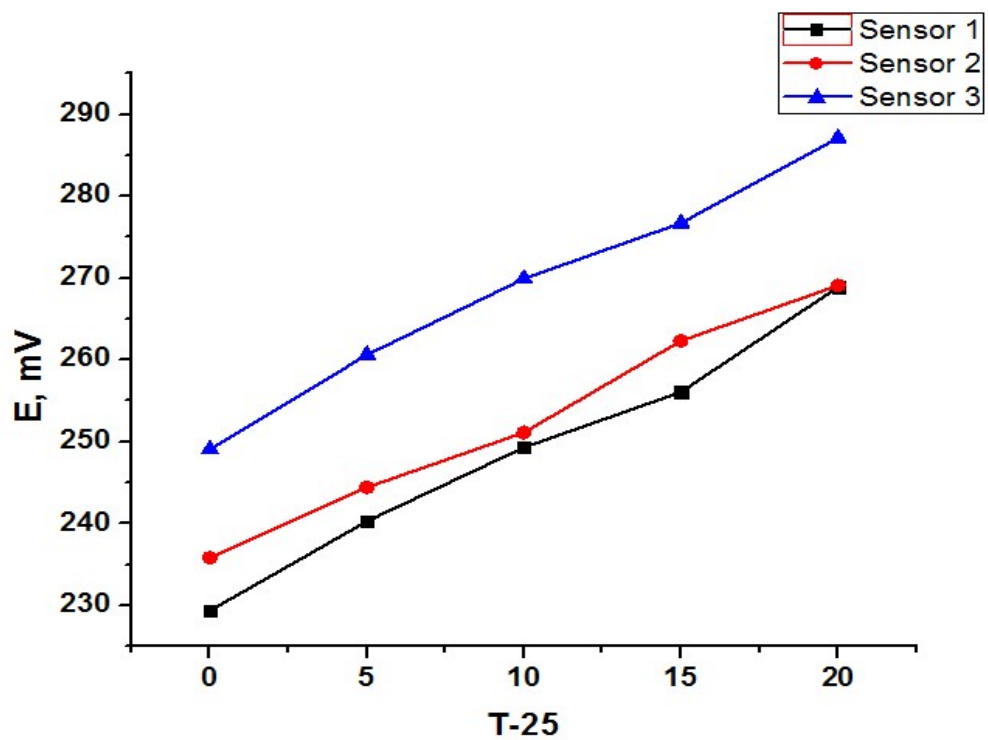


Figure (S2): Variation of standard electrode potential with changes of test solution temperatures for different SPEs.