

Fig.1E

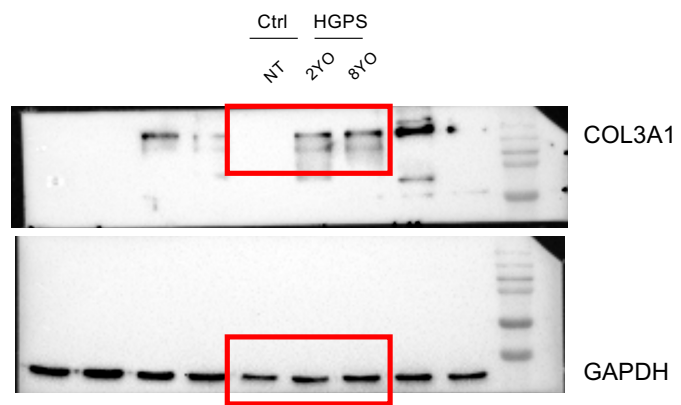


Fig.1F

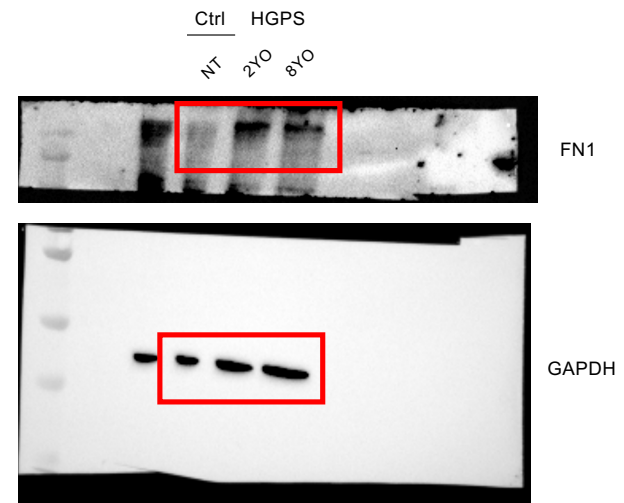


Fig.2C

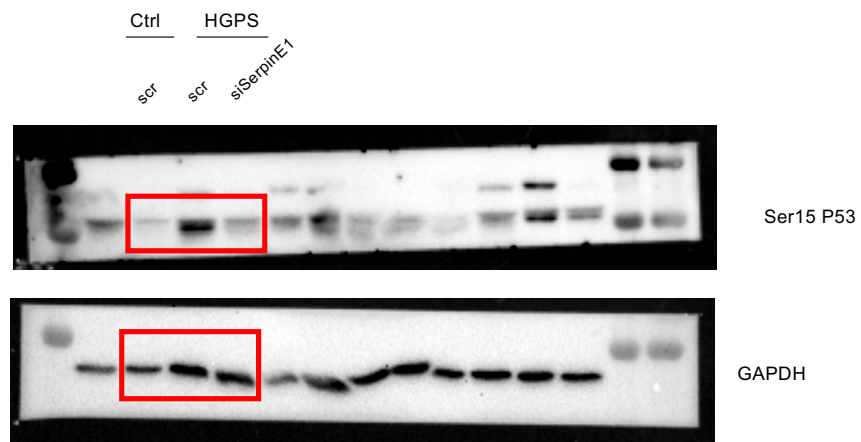


Fig.2G

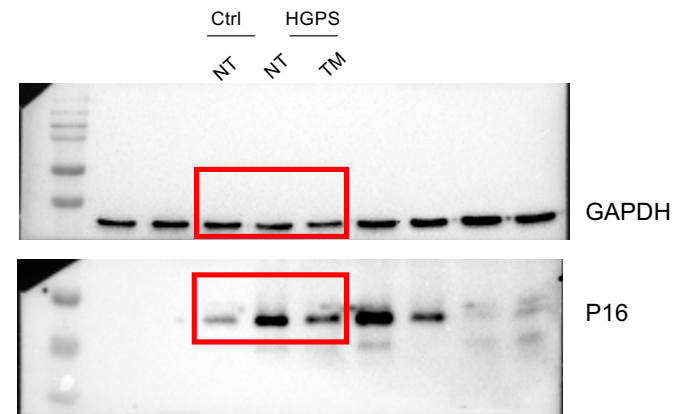


Fig.3A

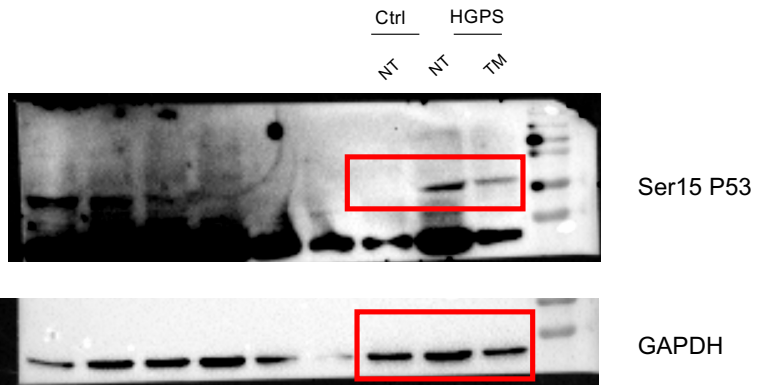


Fig.4E

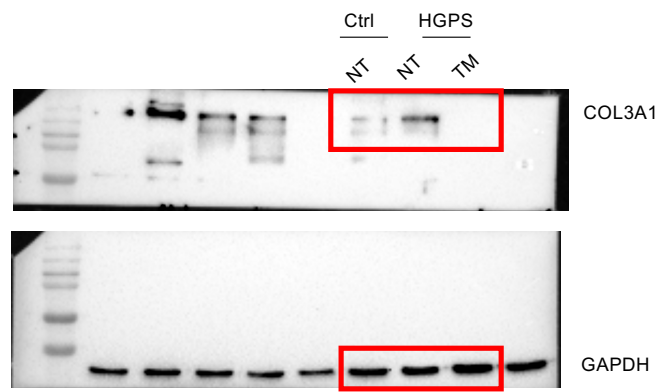


Fig.Supp1C



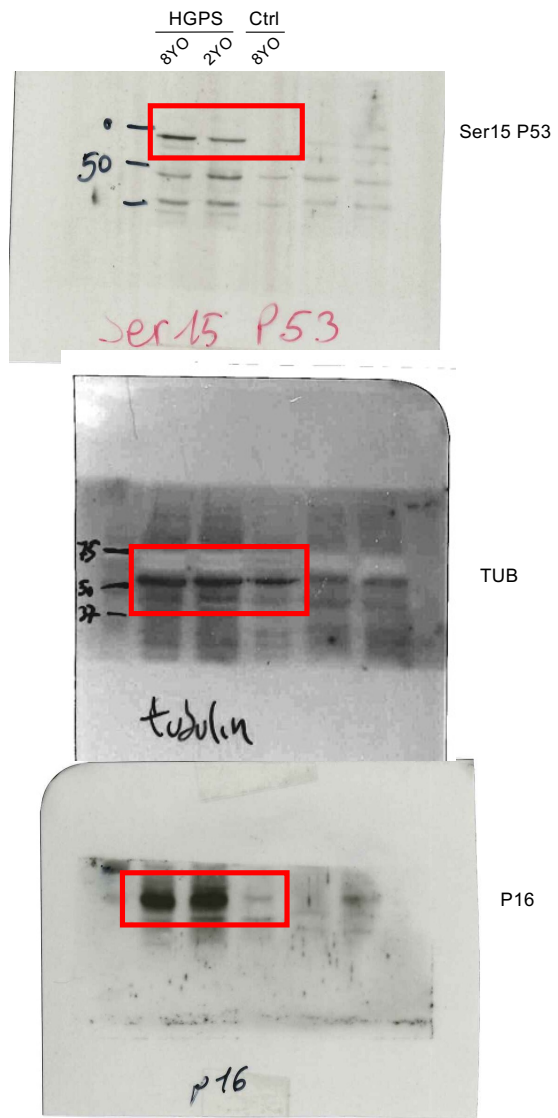



Fig.Supp1D

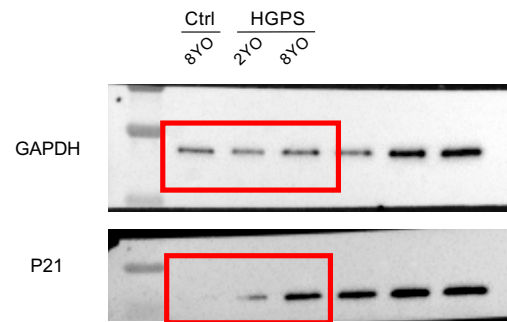

Supp Fig 2B

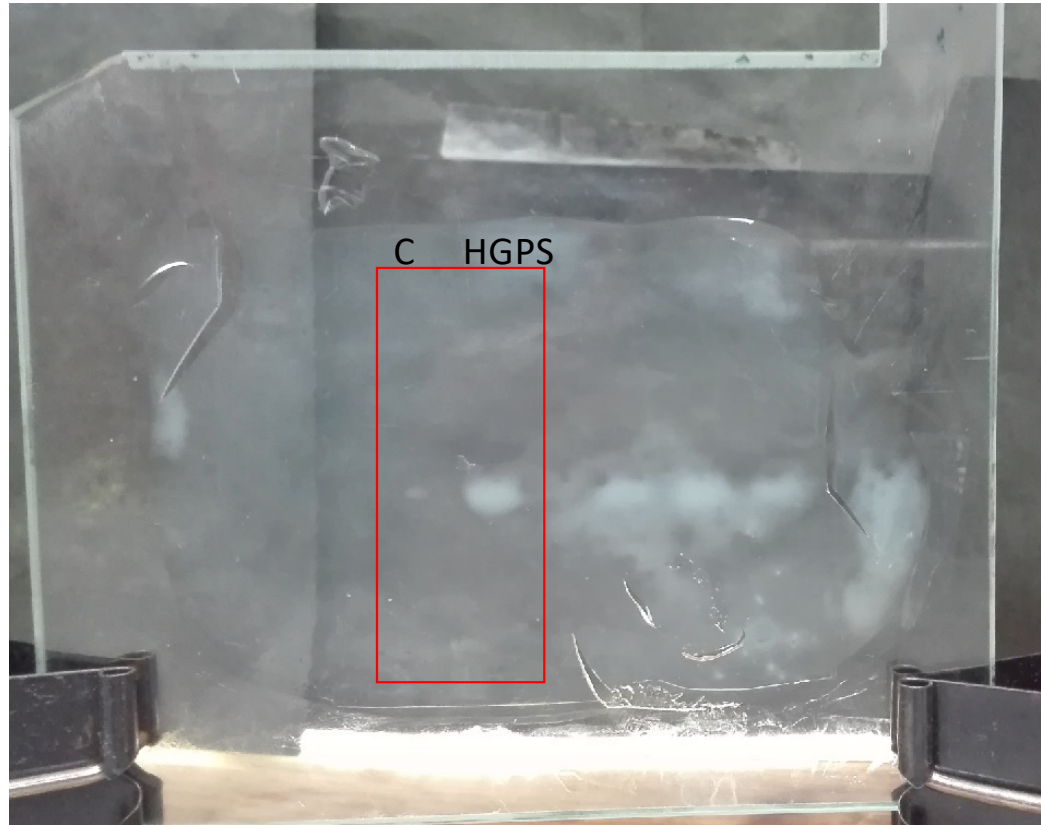



Supp Fig 2C

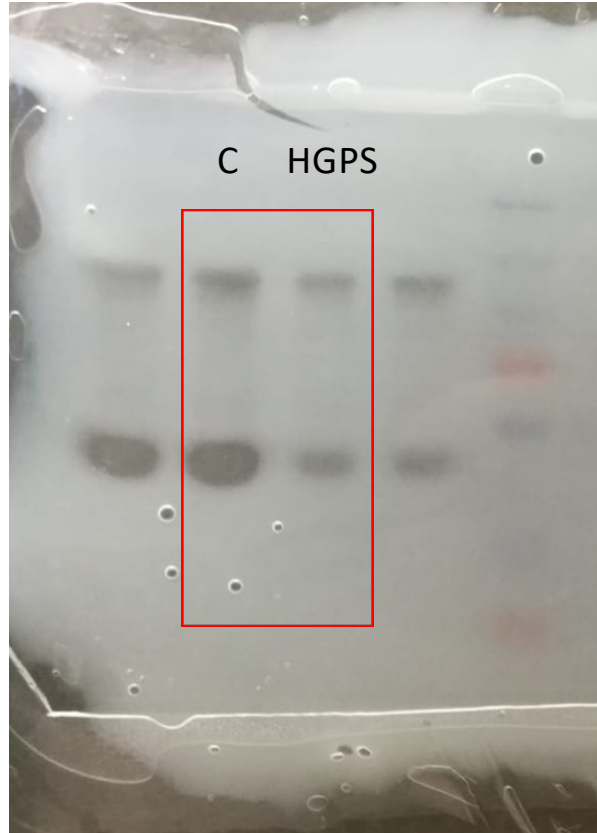

Supp Fig 2E

-Amiloride


+Amiloride

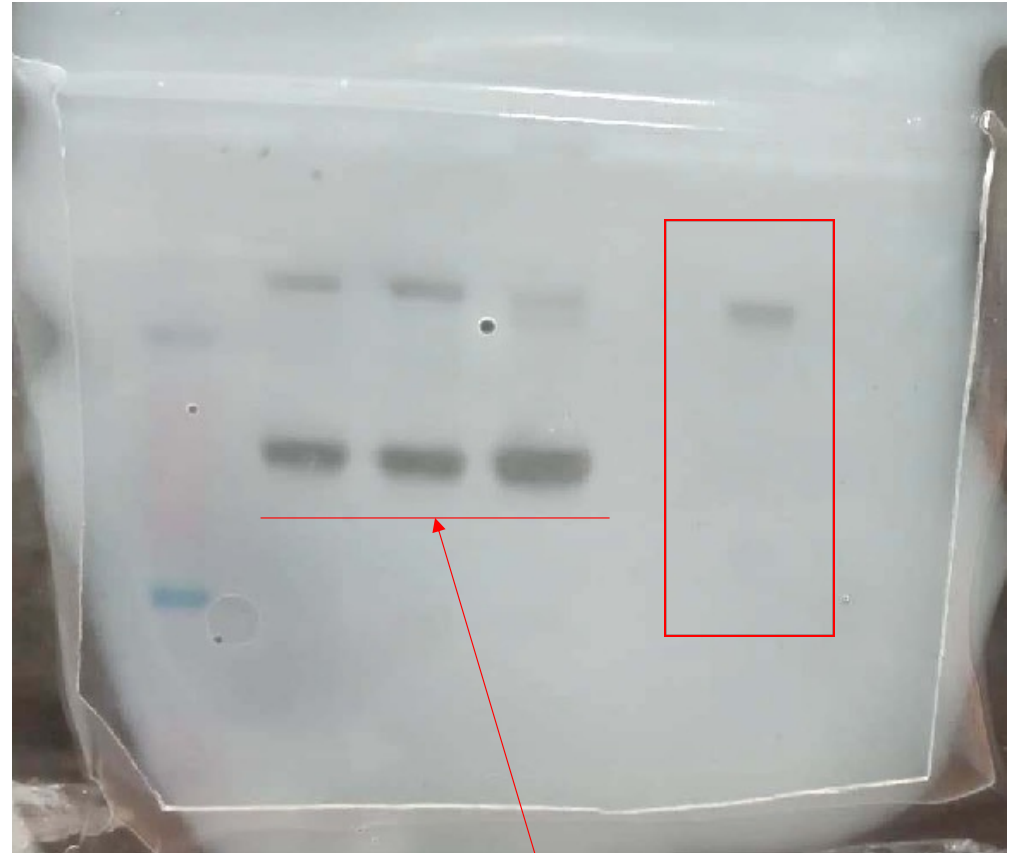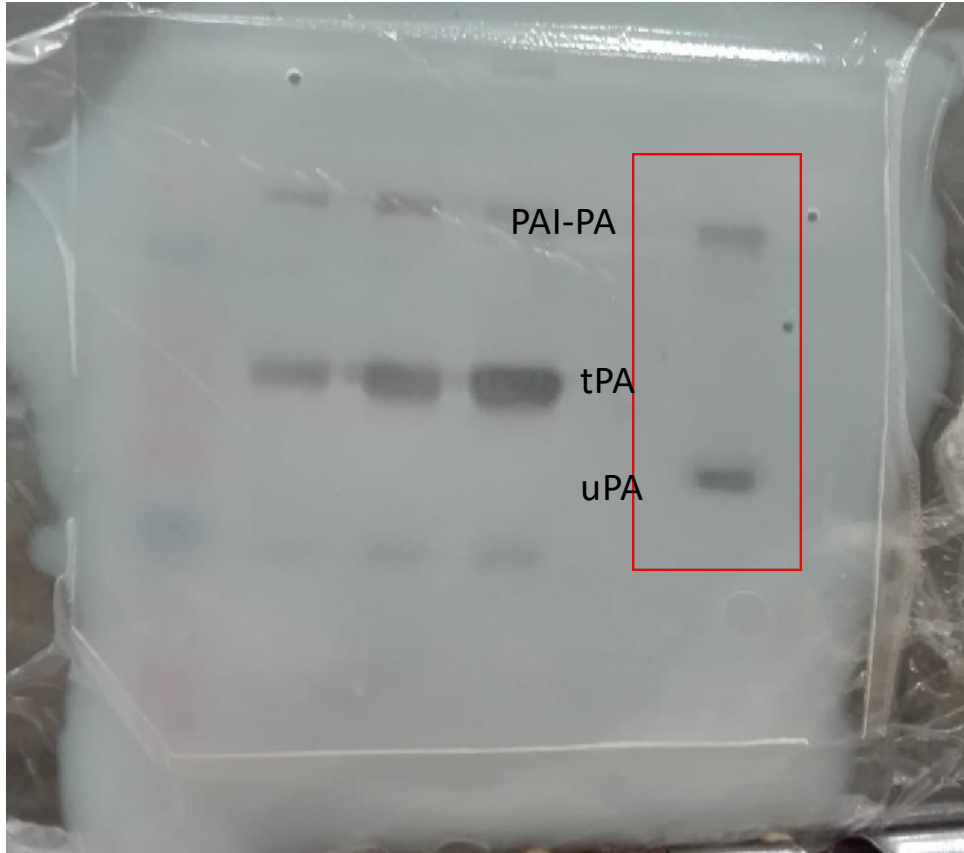

Controls for amiloride  
tPA is not affected by the presence of amiloride



Supp Fig 3A

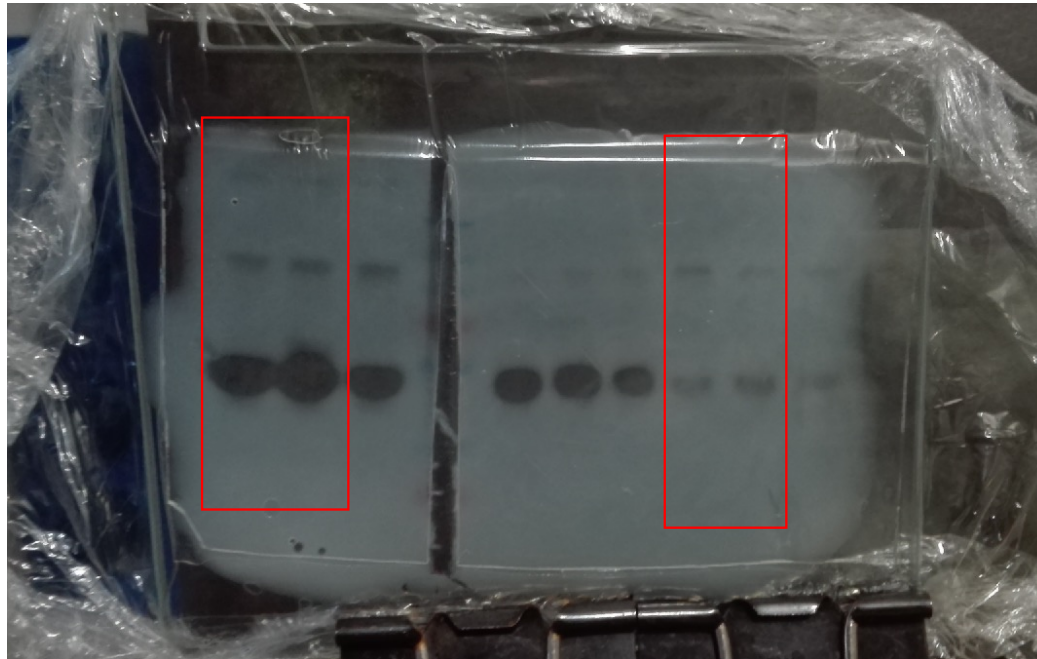

002 2% 002 2% 002 2% 002 2% 002 2% 002 2% Ag 2% Ag 2% Ag 2%  
NT TM10 TM50 NT TM10 TM50 NT TM10 TM50