

Fig. 2B. MDA-MB-468

Supplementary Figures



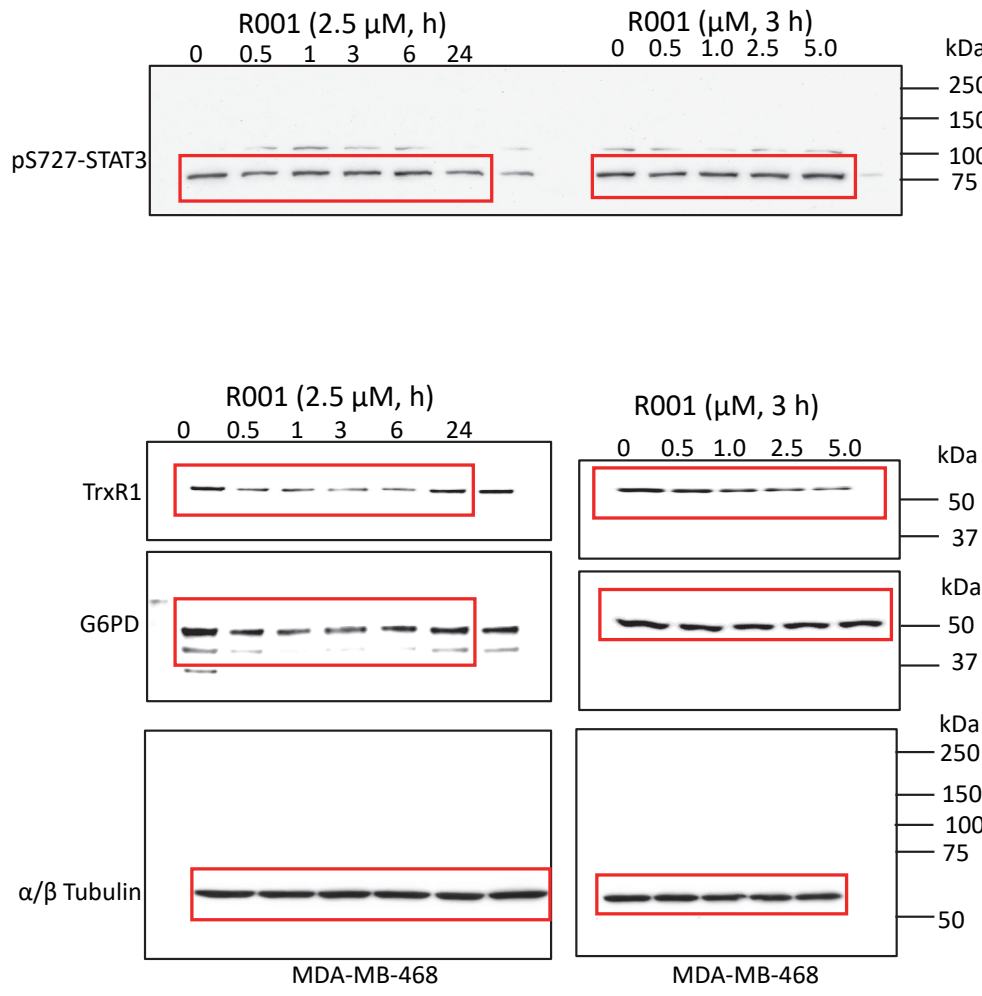




Fig. 2B. MDA-MB-231

Supplementary Figures

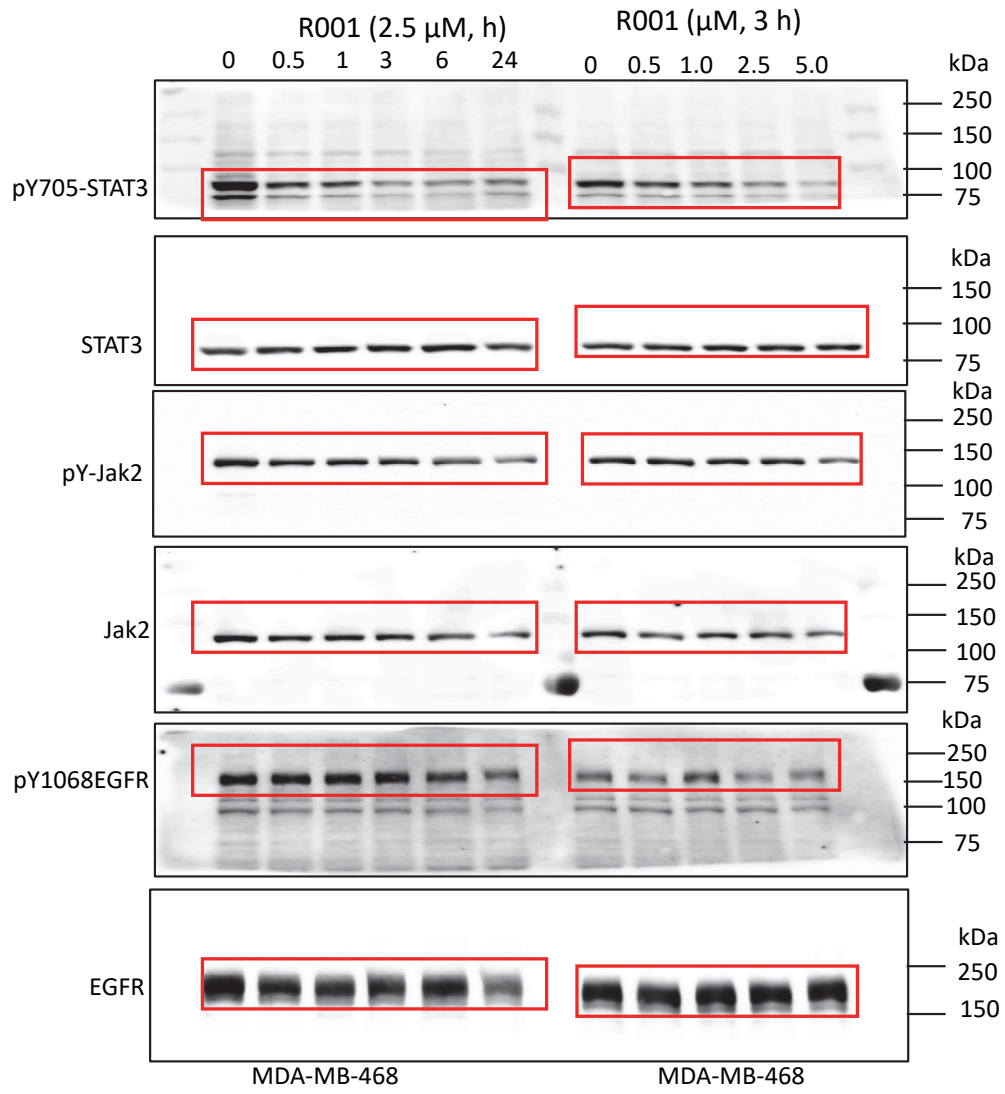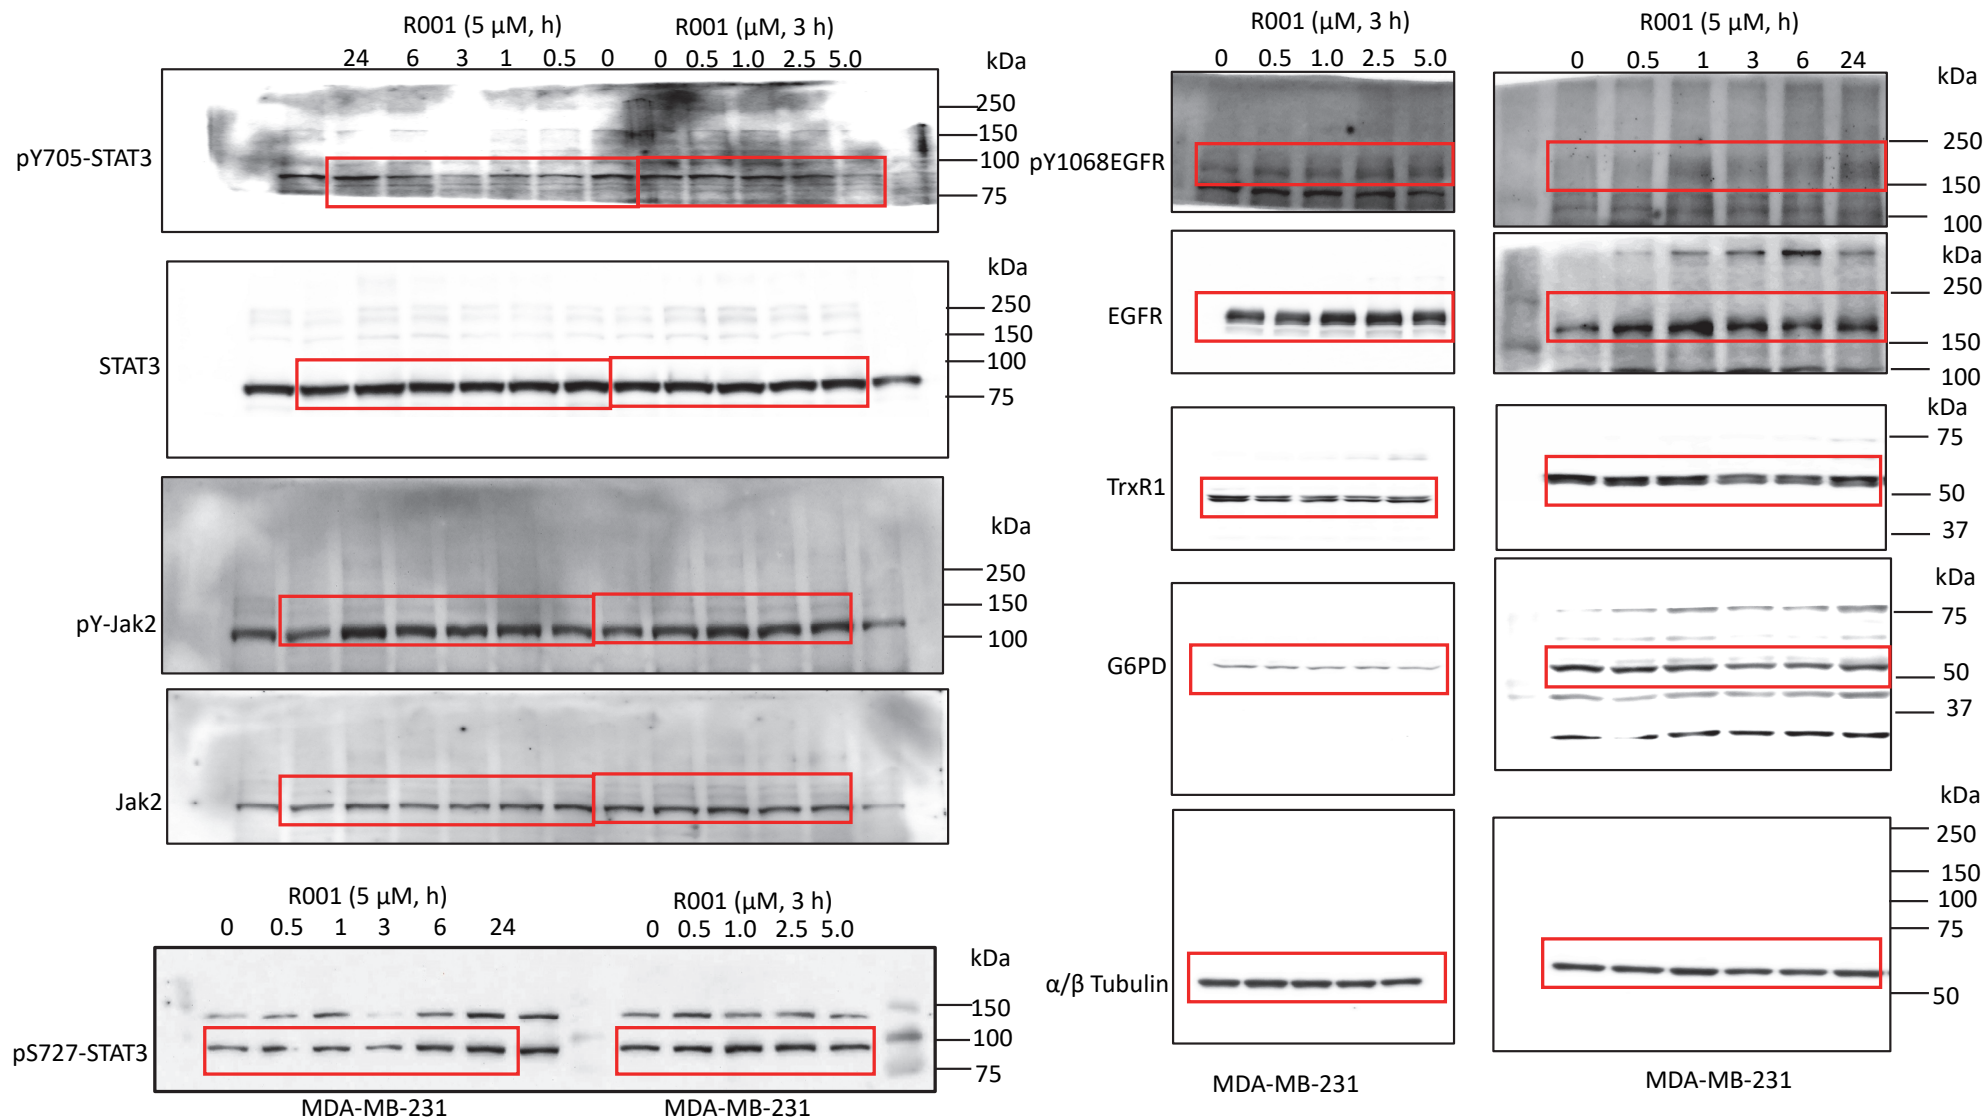

Supplementary Figures

Fig.2C

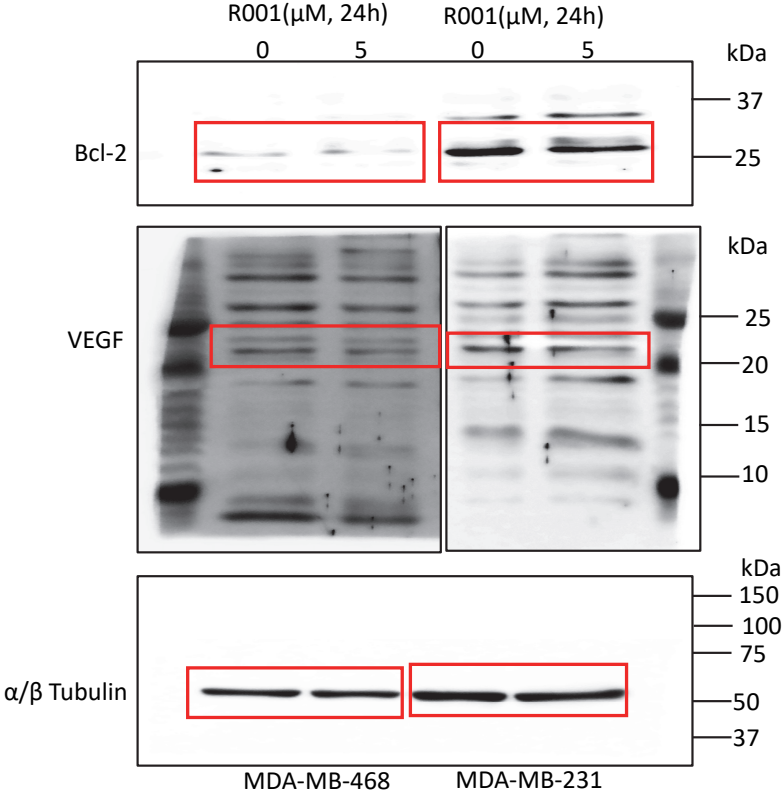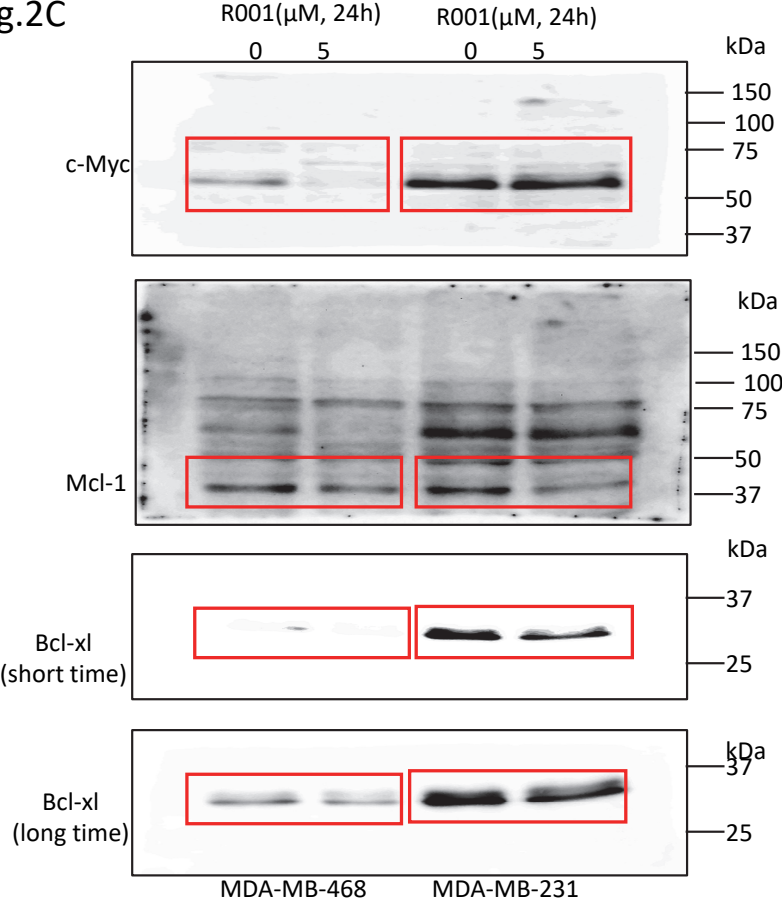

Supplementary Figures

Fig.2D

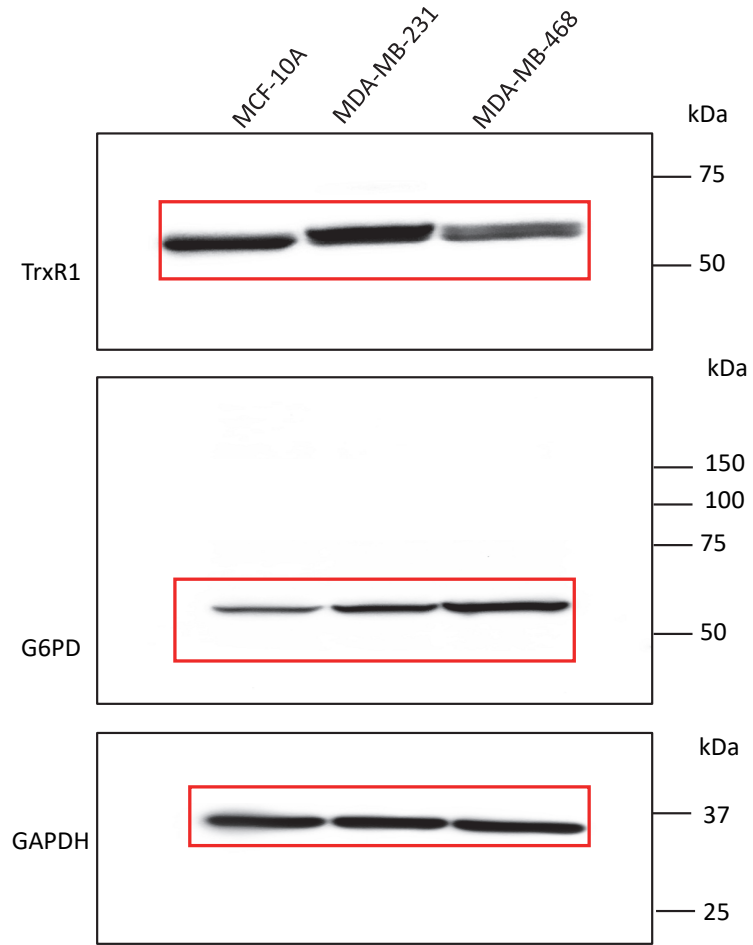


Fig.2G

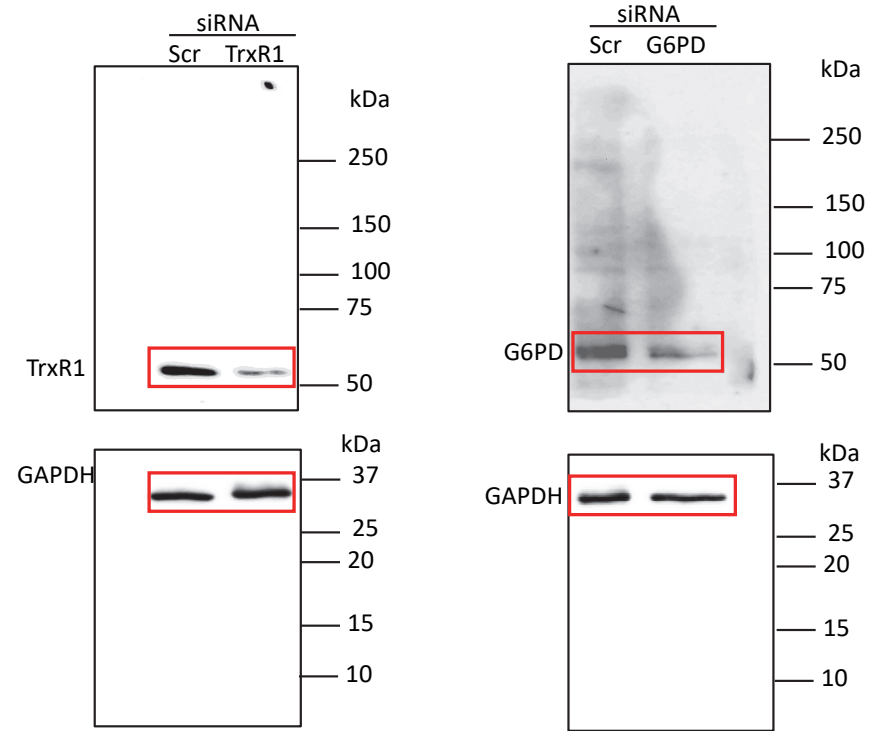


Fig.4C

Supplementary Figures

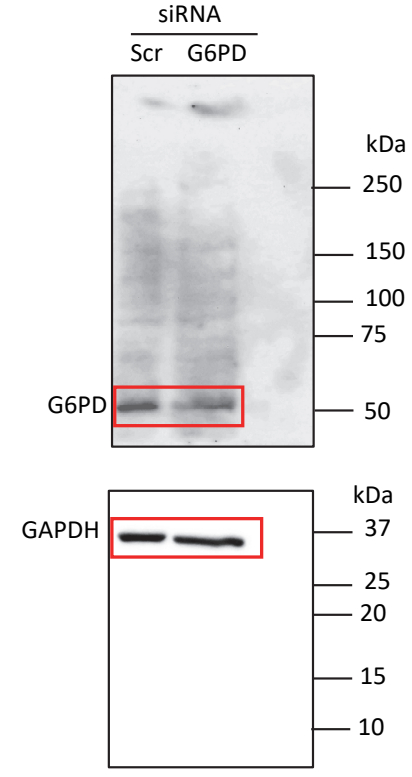
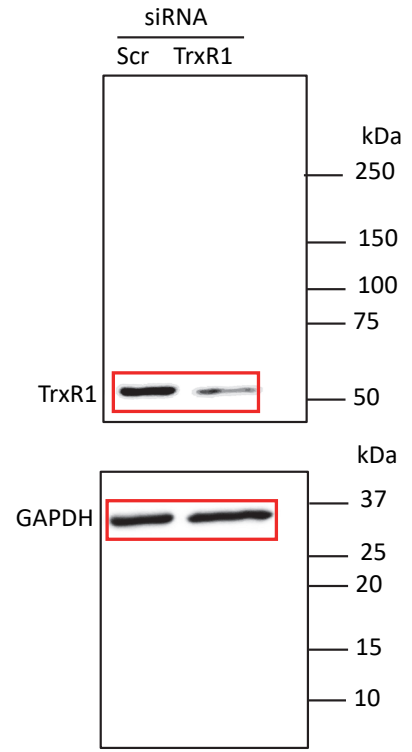
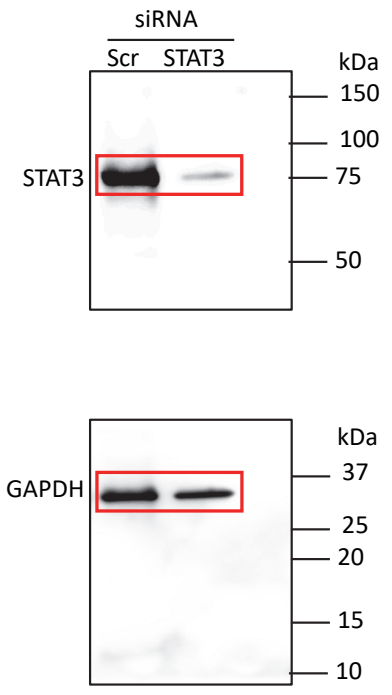


Fig.5A

Supplementary Figures

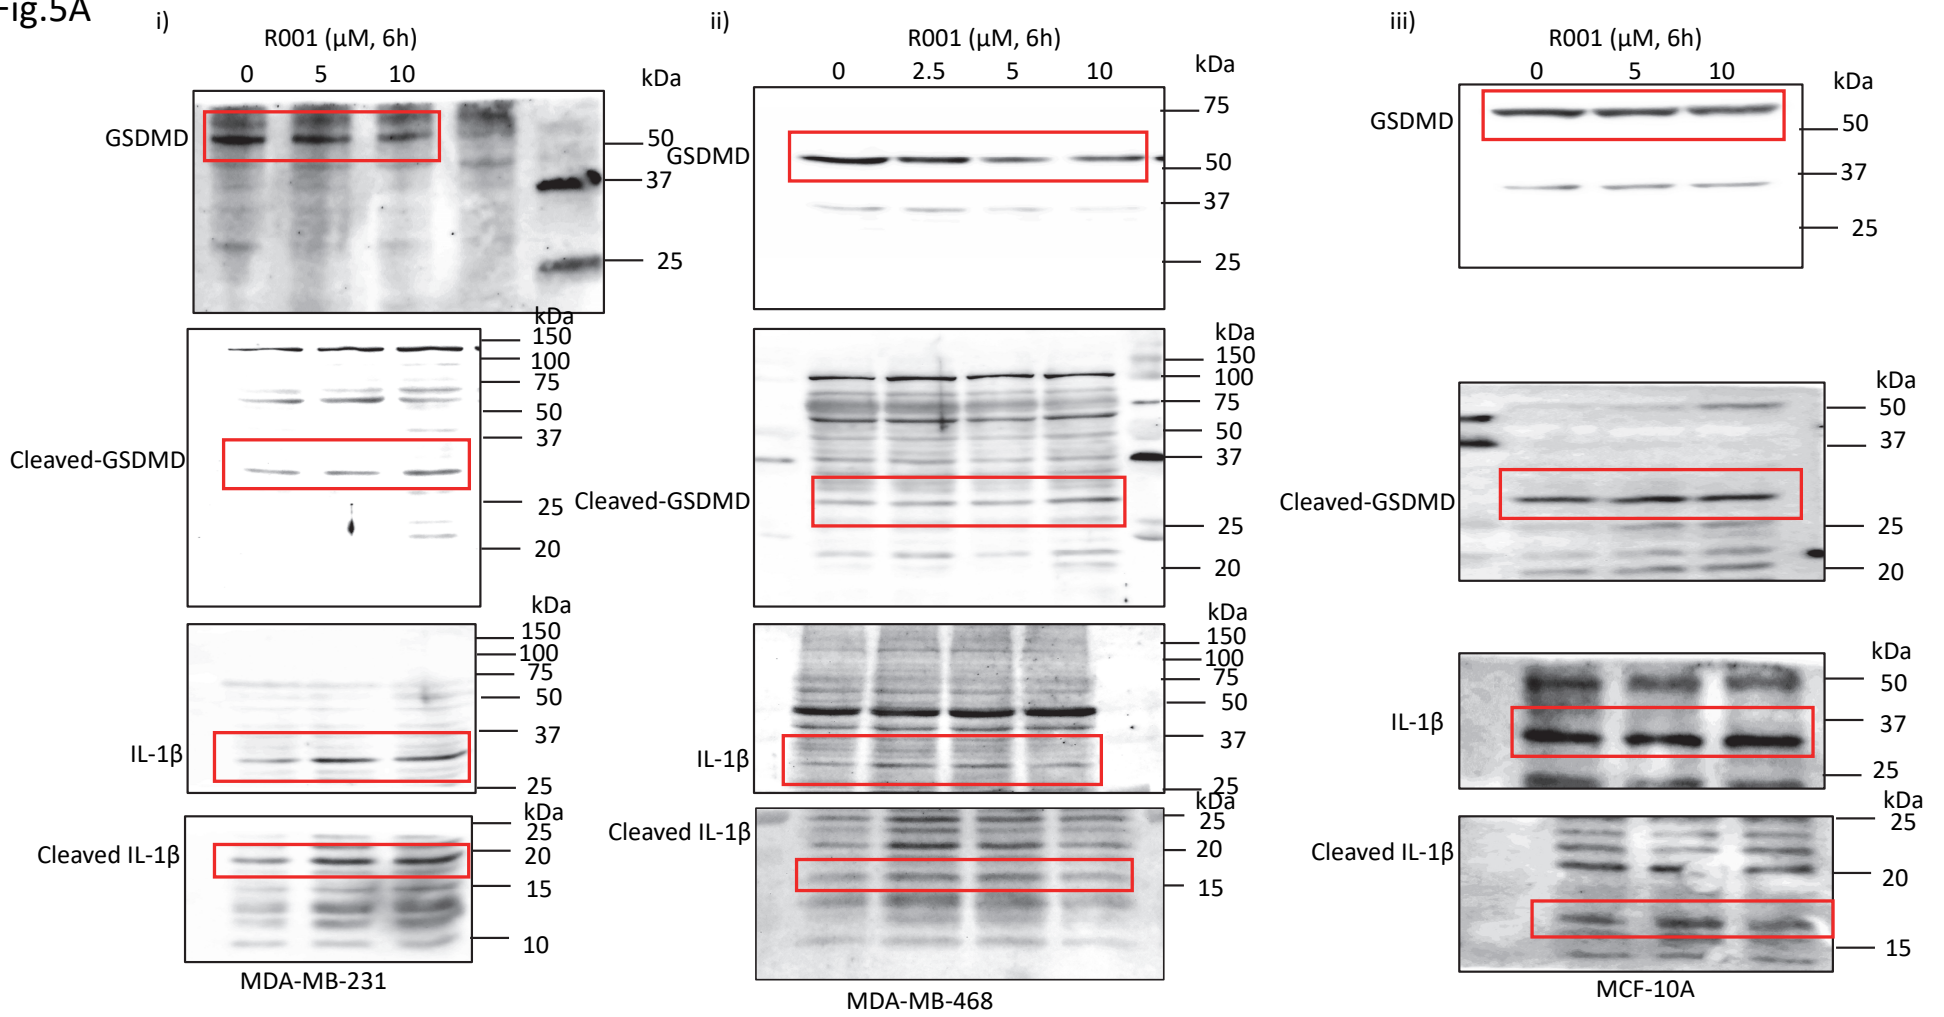


Fig.5A

Supplementary Figures


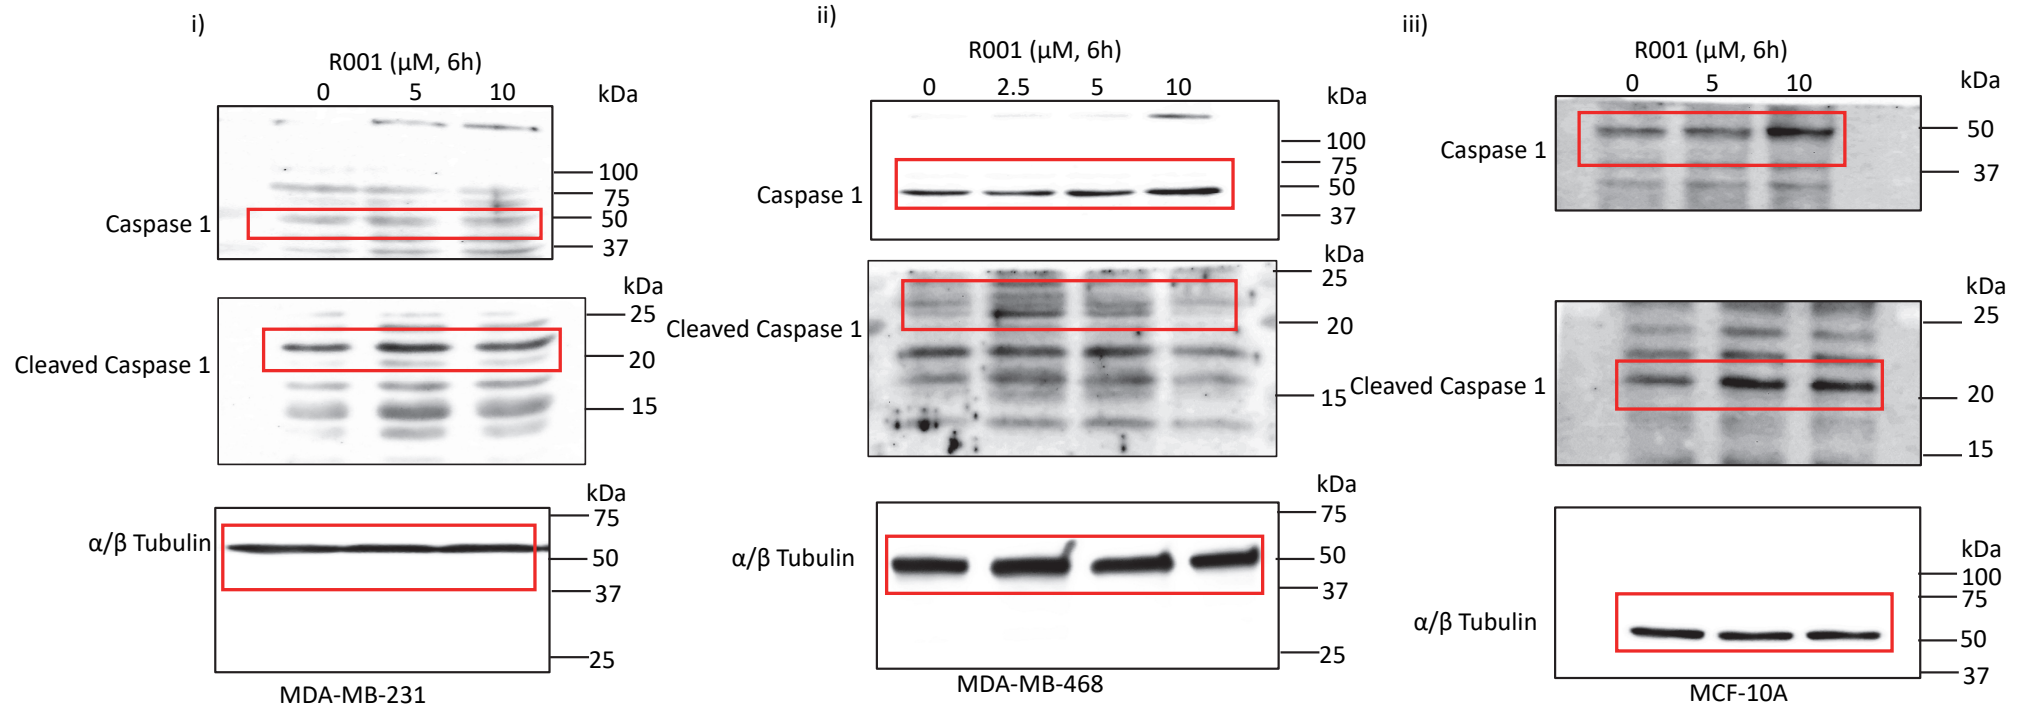


Fig.5F

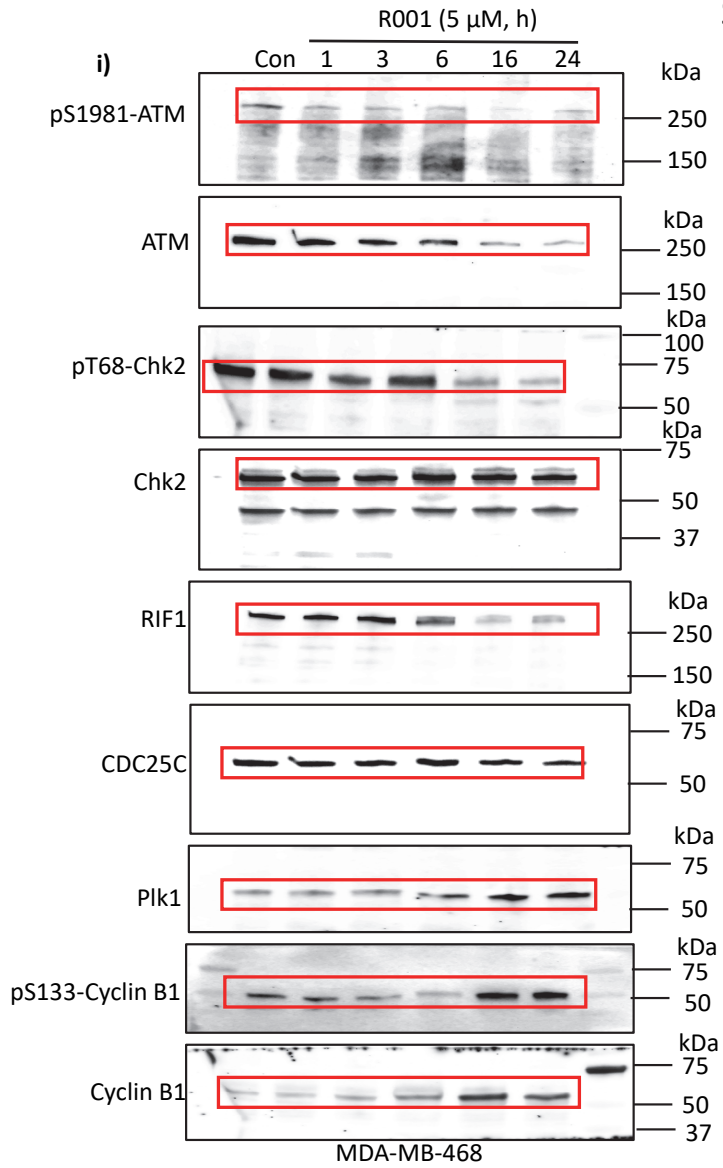

Supplementary Figures

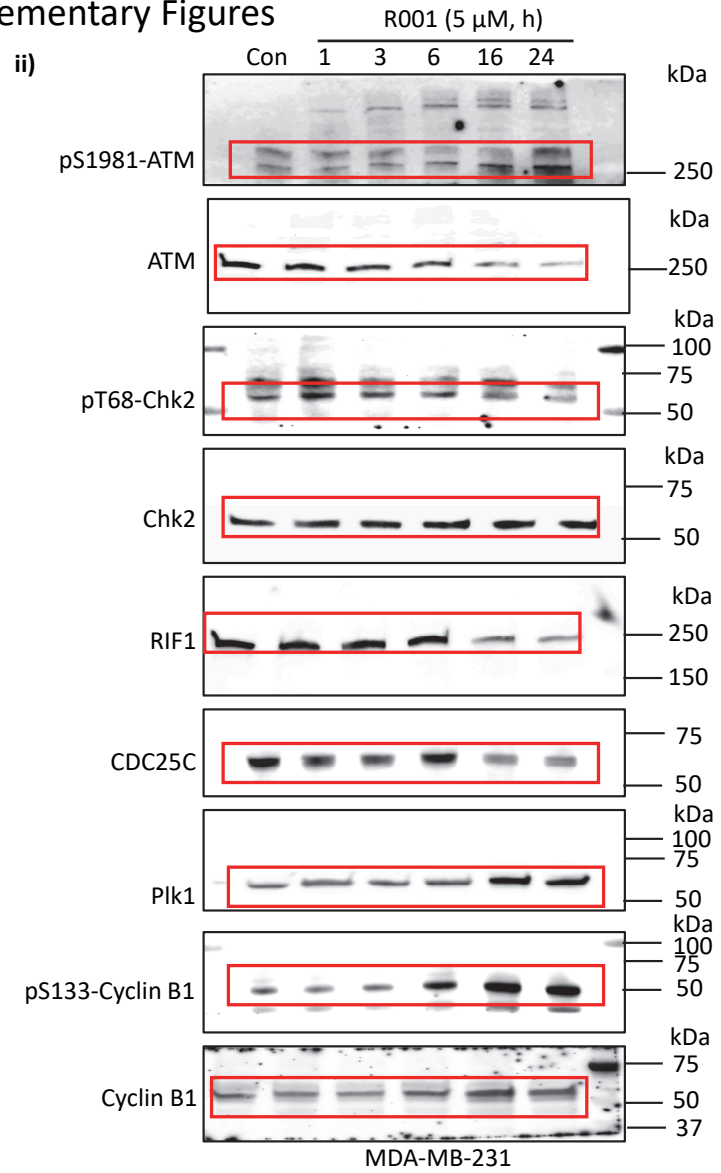


Fig.5F

Supplementary Figures



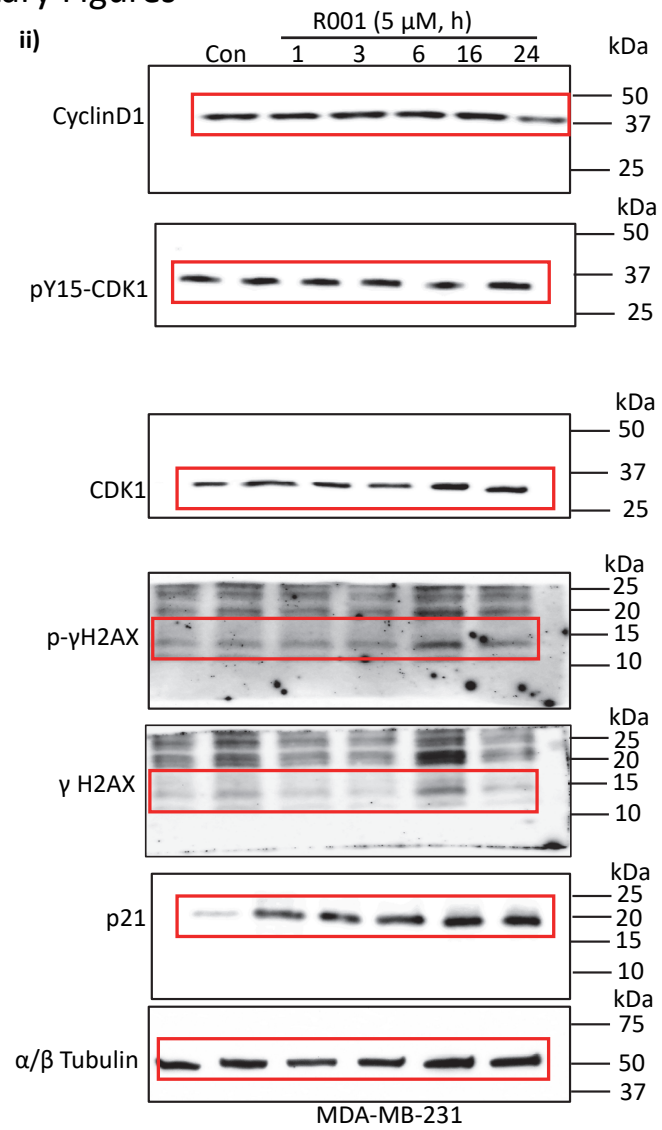


Fig. S2.

Supplementary Figures

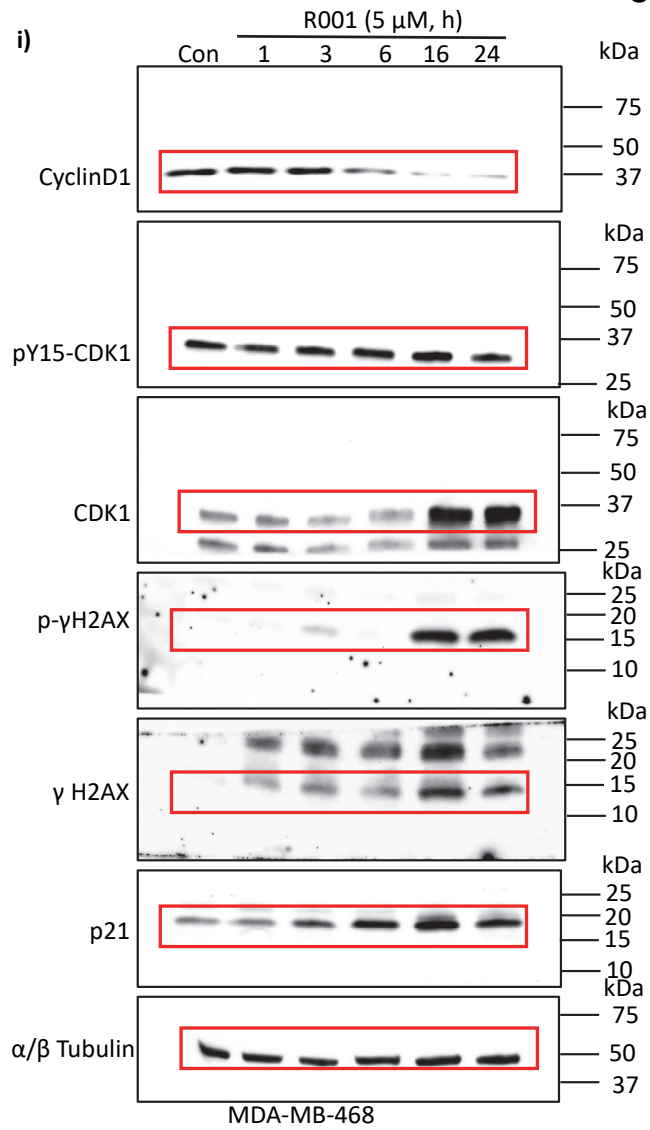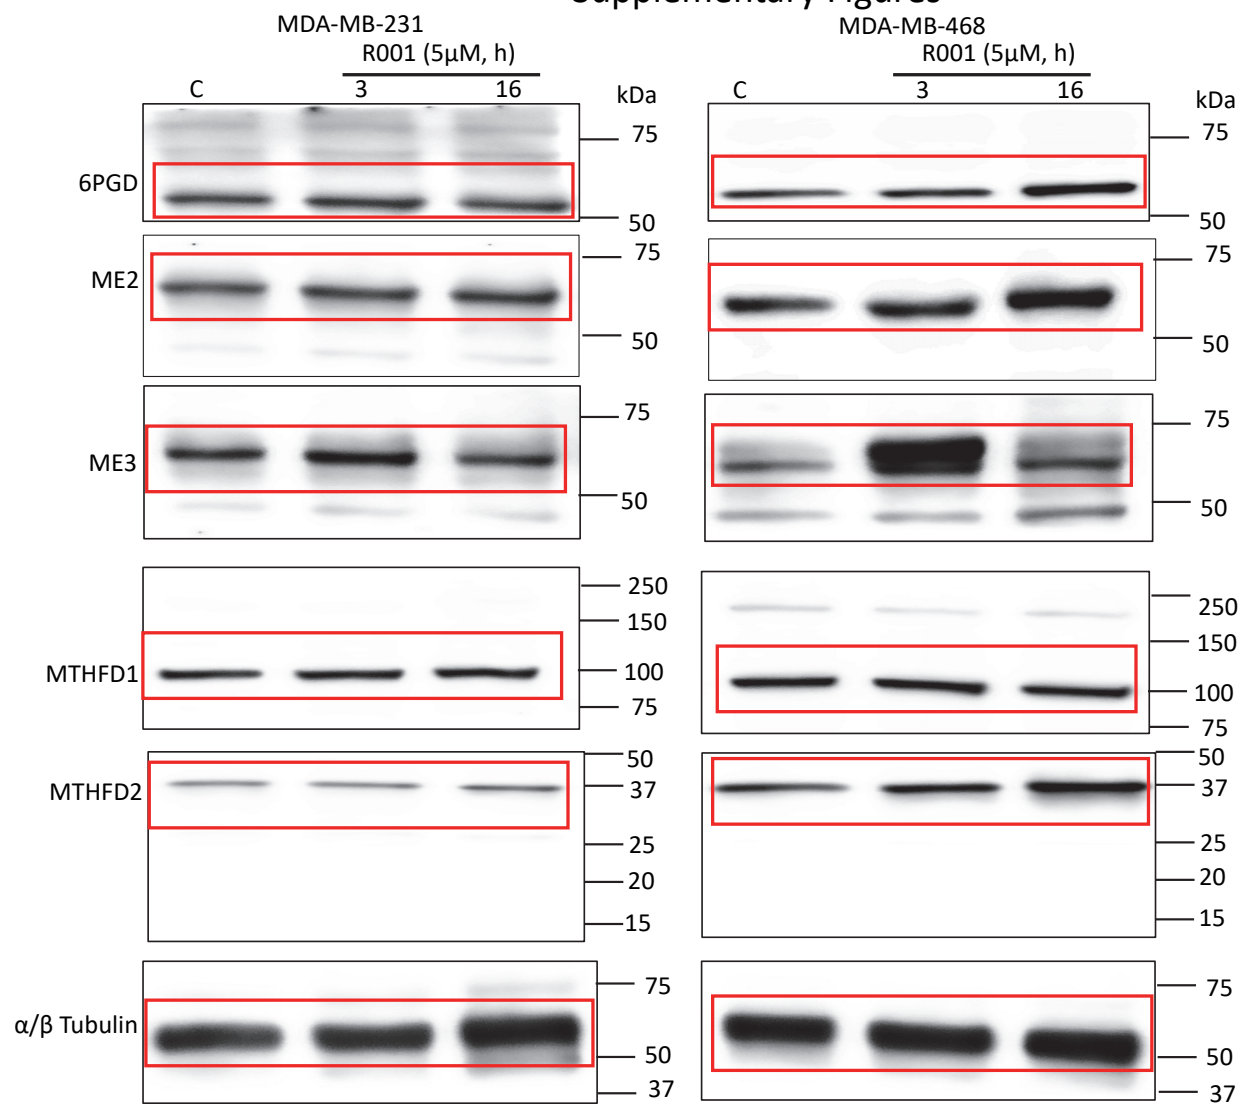

Supplementary Figures

Fig. S6.

