


ImmunoCAP ISAC Assay

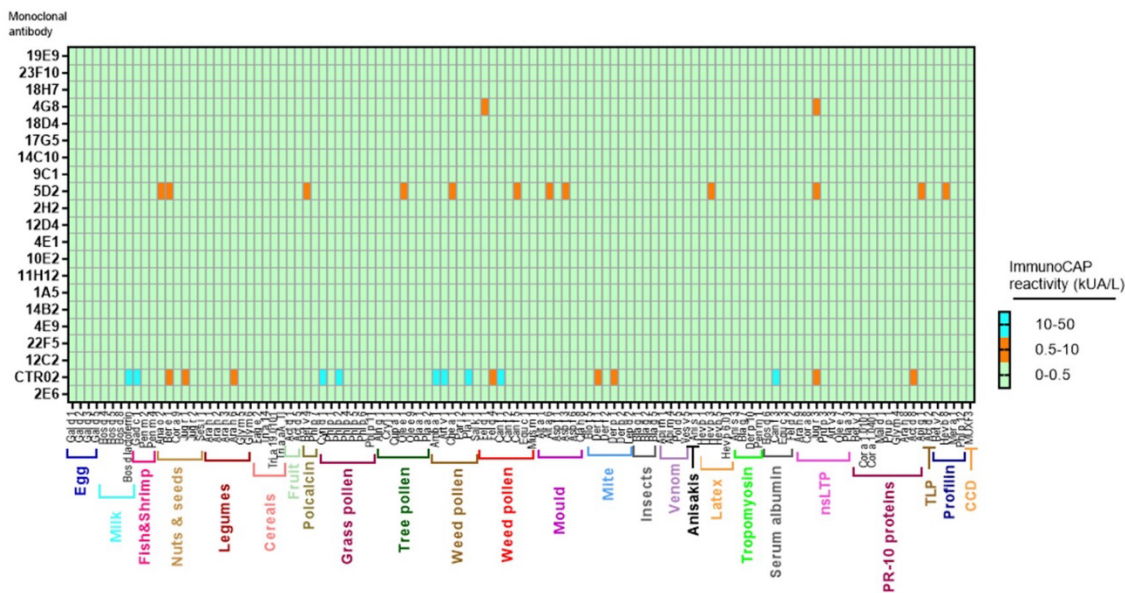

Supplemental Data Figure 2. Cross-reactivity analysis of IgE mAbs from patients with LF against common allergens. Heatmap of IgE binding to an ISAC allergen array. MABs were used at an estimated concentration of 1-10 μ g/mL against 112 common allergens. CTR02 is a positive control included in the immunoCAP ISAC assay.