

M-CSF in Patient Ascites Fluid at Surgery

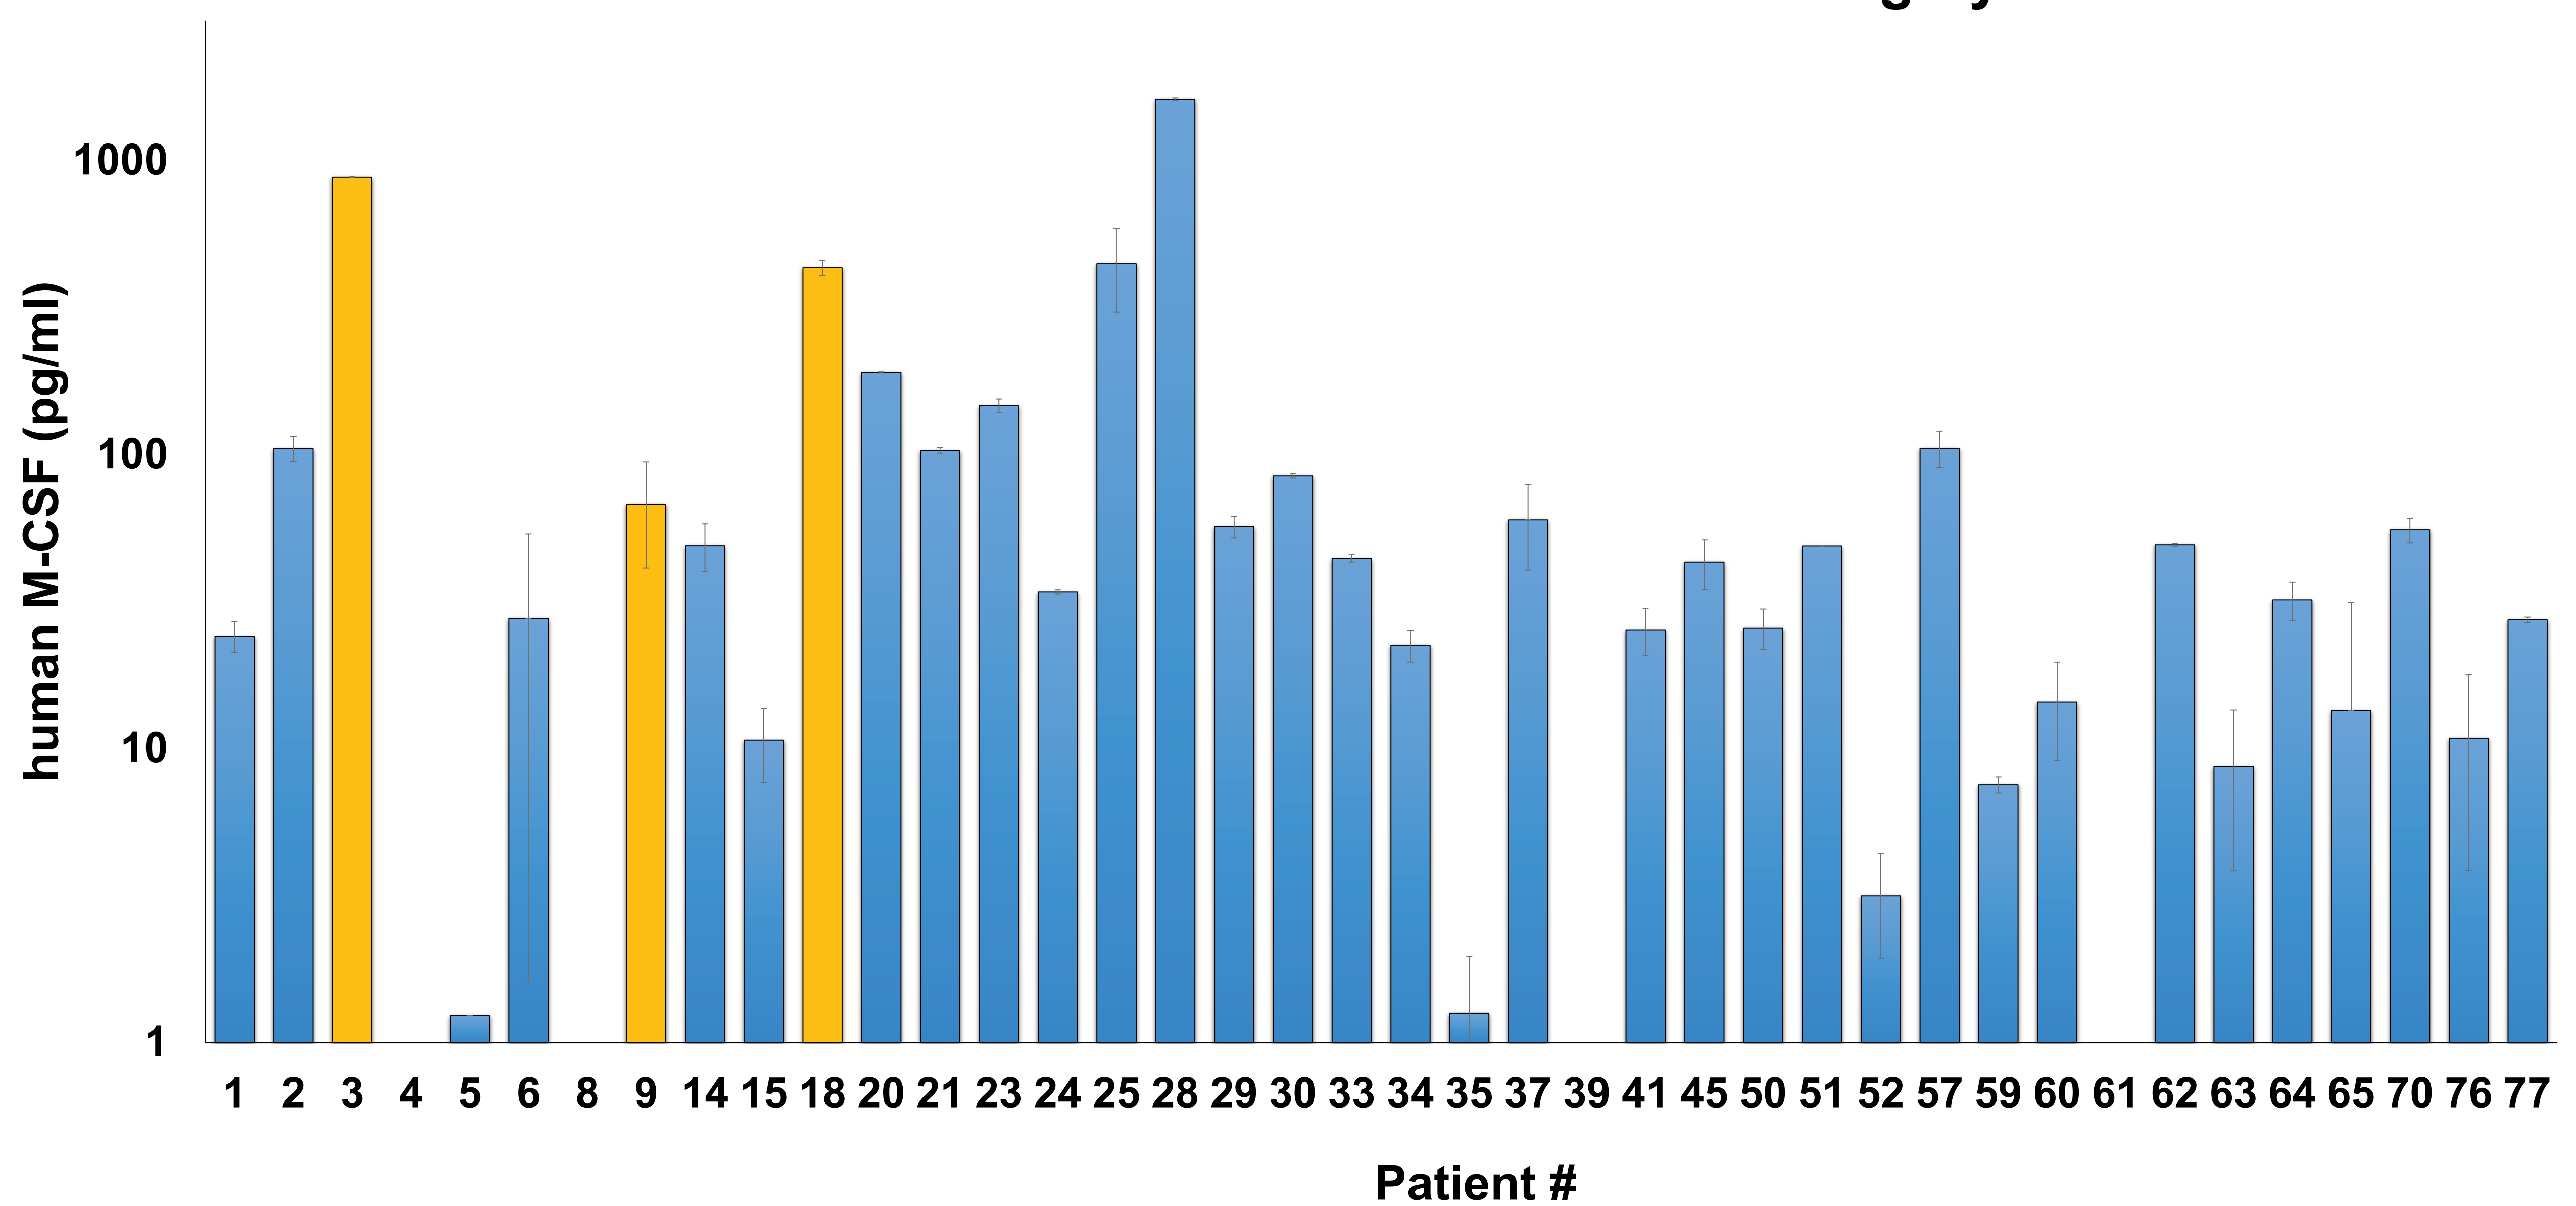


Fig. S4 Levels of human M-CSF detected in patient ascites fluid. Cell-free ascites fluid collected at surgery from 40 ovarian cancer patients was tested for human M-CSF levels by ELISA. Bars are the average of two replicates (+/- STDEV). M-CSF was detectable in 36 of 40 patient samples. Patient samples from which the three PDX used in this study originated are shown in yellow. M-CSF is detectable in 36 of the 40 samples and falls within or above the range of patients 3,9, and 18 in 19 samples.